

**NBSIR 84-2911**

National Bureau of Standards Passive Solar Test Facility - Instrumentation and Site Handbook

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
National Engineering Laboratory
Center for Building Technology
Building Equipment Division
Gaithersburg, MD 20899

June 1984

Issued August 1984

Prepared for:

U.S. Department of Energy
Office of Solar Heat Technologies
Passive and Hybrid Solar Energy Division
Experimental System Research Program
Washington, DC 20585

QC

100

.456

no. 84-2911

1984

C.2

NBSIR 84-2911

**NATIONAL BUREAU OF STANDARDS
PASSIVE SOLAR TEST FACILITY -
INSTRUMENTATION AND SITE
HANDBOOK**

Bal M. Mahajan

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
National Engineering Laboratory
Center for Building Technology
Building Equipment Division
Gaithersburg, MD 20899

June 1984

Issued August 1984

Prepared for:
U.S. Department of Energy
Office of Solar Heat Technologies
Passive and Hybrid Solar Energy Division
Experimental System Research Program
Washington, DC 20585



U.S. DEPARTMENT OF COMMERCE, Malcolm Baldrige, *Secretary*
NATIONAL BUREAU OF STANDARDS, Ernest Ambler, *Director*

ABSTRACT

The National Bureau of Standards (NBS), under the sponsorship of the U.S. Department of Energy (DOE) has constructed a passive solar test facility. As a part of the DOE's Experimental Systems Research Program, the NBS test facility has been constructed for the purpose of acquiring and distributing to participating researchers class A level performance data for different passive systems. These data are acquired for use in: detailed building energy analysis and model/algorithm validation; and performance characterization of passive subsystems.

This handbook provides a complete description of the test building, thermo-physical properties of the building material, location of the sensors installed at the test facility, and data acquisition system and procedures.

NOTES FOR THE FIGURES

1. All dimensions shown in the figures are nominal.
2. The test facility was constructed using the nominal dimensions in English Units. Expression of the dimension in Metric Units would suggest inordinately small dimensional tolerances. Hence the dimensions are shown in English Units. For the convenience of the readers, the Metric equivalent of English Units are given below.

1 foot = 0.3048 meter

1 inch = 0.0254 meter

TABLE OF CONTENTS

	<u>Page</u>
1. INTRODUCTION	1
2. GENERAL ENVIRONMENTS	3
3. DESCRIPTION OF THE BUILDING	5
3.1 General	5
3.2 Ceiling/Roof	8
3.3 Floor	8
3.4 Walls	12
3.5 Windows	18
3.6 Individual Cells	18
3.7 Material Properties and Heat Loss Coefficient of Test Cells	33
3.8 Auxiliary Heating and Cooling System	33
4. INSTRUMENTATION	37
4.1 Outside	37
4.2 Cell #1	41
4.3 Cell #2	41
4.4 Cell #3	48
4.5 Cell #4	48
5. DATA ACQUISITION AND DISTRIBUTION	58
5.1 Data Acquisition System	58
5.2 Continuous Air Infiltration Monitoring System	58
5.3 Data Acquisition and Distribution	59
5.4 Estimates of Uncertainty in the Measured Data	59
6. CONCLUDING REMARKS	63
7. ACKNOWLEDGEMENT	63
8. REFERENCES	64
8. APPENDIX A. A Copy of Data Documentation	66

1. INTRODUCTION

In 1980, the U.S. Department of Energy established a Program Area Plan for systematic performance evaluation of passive/hybrid heating and cooling systems [1, 2]. This program area plan defines three levels of performance monitoring procedures which, in decreasing order of sophistication, have been designated as Class A, B, and C. Both class A and class B level monitoring involved fixed instrumentation and data acquisition equipment, while class C level monitoring involves simple hand-recorded measurements and surveys of occupant reactions.

Class B level monitoring provides limited detailed data (about 20 sensors per building) from occupied buildings for field testing and statistical evaluation of passive systems and buildings. Class A level monitoring is defined to provide carefully measured detailed data (about 200 sensors per building) under controlled conditions for use in (1) detailed building energy analysis and model/algorithm validation; and (2) performance characterization of various passive subsystems.

The National Bureau of Standards (NBS), under the sponsorship of DoE, has constructed a full-scale four-cell passive solar test facility. The test facility contains several types of generic passive solar features such as a direct gain system, a collector storage wall (Trombe wall), and clerestory windows. The NBS test facility has been constructed as a part of the DoE's Experimental Systems Research Program and is used for acquiring and distributing to participating researchers class A level performance data for various passive subsystems under different experimental conditions. The purpose of this handbook is to provide to the data users (i.e. models, algorithms developer/validators) a complete physical description of the test building as well as the location of sensors used for gathering data.

The test facility was made operational in October of 1981, with the direct gain cell completely instrumented and the other cells minimally instrumented. A handbook describing the NBS test facility, thermophysical properties of construction materials, and sensor locations was published and distributed [3]. During FY82 performance data from the direct gain cell, under three different experimental conditions, were collected and distributed to the participating researchers. A technical paper containing the representative results from these data was presented at the ASME Passive Solar Division Sixth Annual Technical Conference in April 1983 [4].

In FY83 instrumentation of the Trombe wall cell was completed. A new data acquisition system (DAS) and a multichannel continuous air infiltration monitoring system (CAIMS) were procured and installed at the test facility. During FY83 some experiments were conducted to monitor the performance of the direct gain and Trombe wall cells, and to measure the thermocirculation characteristics of the Trombe wall. A paper containing a brief description of the new DAS and CAIMS, and some representative results from the FY83 experimental work was presented at the Passive and Hybrid Solar Energy Update meeting in September 1983 [5]. The data tape containing the hourly average data set was distributed

to the participating researchers. In the beginning of FY84 some additional thermocouples were installed in the direct gain cell (cell #4) and the control cell (cell #3).

This handbook contains a complete physical description of the test facility, as well as the thermophysical properties of the building materials and building components. The handbook contains a complete directory (type and location) of the sensors installed in and around the building, and a brief description of DAS and CAIMS. The handbook also describes the data acquisition procedures and estimates of uncertainty in the measured data.

2. GENERAL ENVIRONMENTS

A site plan for the NBS Passive Solar Test Building is given in figure 1. Note that the contour slopes downward from south to north at the building site. Grass surrounds the building except for the concrete walkway and blacktop drive. Immediately to the south, a coarse gravel bed (reflectance ≈ 0.2) extends out 1.12 m (3.67 ft) from the south wall. Beyond that, the ground is rocky earth with sparse grass (reflectance = 0.2). During the winter, this area is sometimes covered with snow (reflectance = 0.7). There is no significant shading effect from trees or other external objects.

The American Institute of Architects Research Corporation (AIA/RC) regional climatic classification for Washington, DC, is type 7A (Atlantic Coast).^{*} The annual number of heating degree days is 2347°C-days (4224°F-days), the average winter temperature is 7.6°C (45.7°F), and the 97.5 percent design dry-bulb temperature for heating is 8.3°C (17°F). The annual number of cooling degree days is 522°C-days (940°F-days), and the 2.5 percent design dry-bulb and mean coincident wet-bulb temperatures are 32.8°C (91°F) and 23.3°C (74°F), respectively. Annual average wind speeds are medium [11 to 24 km/h (7 to 15 mph)] and prevailing winds are from the southwest. Cloud cover is 0.65 to 0.75 from December to March and 0.55 to 0.65 for the rest of the year. The nearest Typical Meteorological Year weather station is at the Dulles International Airport in Sterling, VA.

Monthly rain and snowfall figures for National Airport, Washington, DC, are as follows (suitable figures were not available for Dulles International Airport):

	Rain		Snow	
	<u>cm</u>	<u>in.</u>	<u>cm</u>	<u>in.</u>
January	6.7	2.6	11.4	4.5
February	6.2	2.5	12.7	5.0
March	8.5	3.3	6.1	2.4
April	7.3	2.7	trace	-
May	9.8	3.7	trace	-
June	8.8	3.5	0	0
July	10.5	4.1	0	0
August	11.9	4.7	0	0
September	7.8	3.1	0	0
October	6.8	2.7	trace	-
November	7.4	2.9	1.8	0.7
December	7.6	3.0	9.7	3.8
Annual	<u>99.3</u>	<u>38.8</u>	<u>41.7</u>	<u>16.4</u>

* "Regional Guidelines for Building Passive Energy Conserving Homes," prepared by the AIA/RC for the U.S. Department of Housing and Urban Development, HUD-PDR-355 November 1978, p. 125.

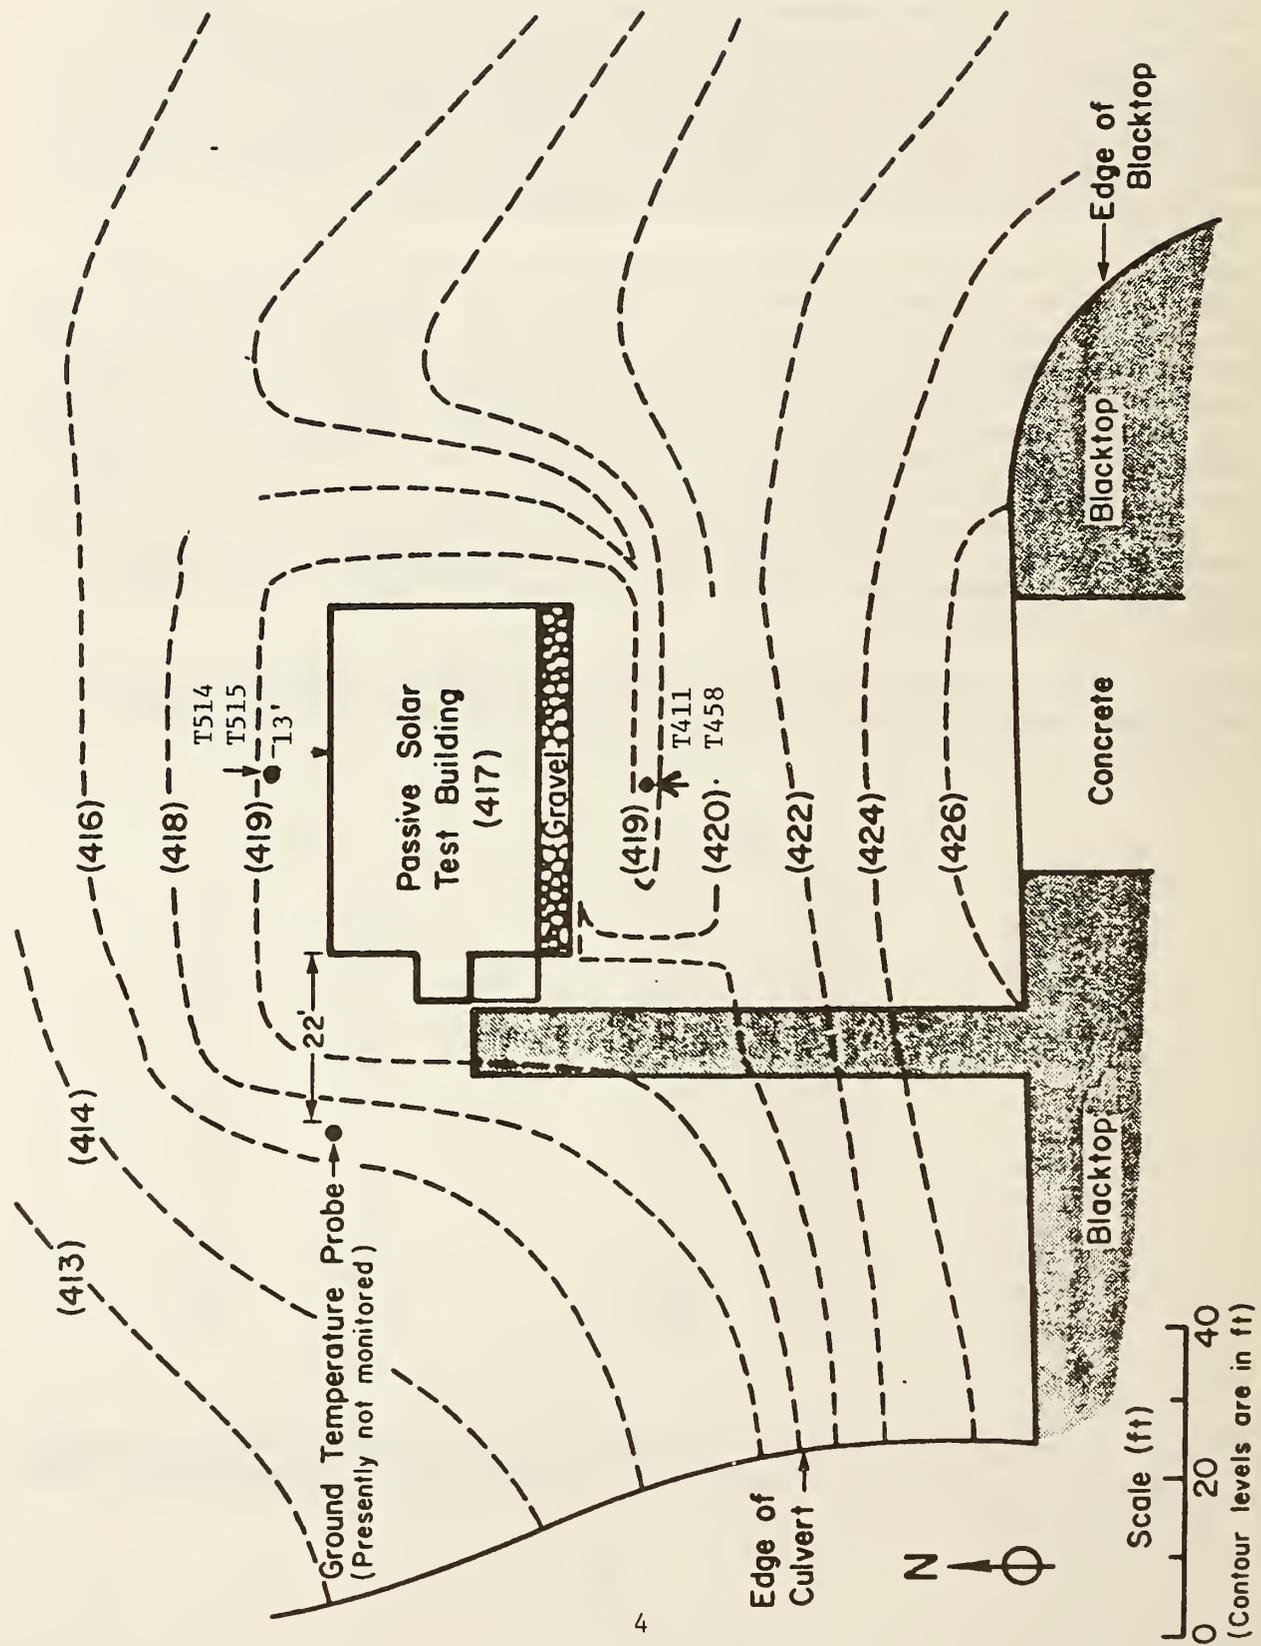


Figure 1. Site Plan of the NBS Passive Test Building

3. DESCRIPTION OF THE BUILDING

3.1 GENERAL

The NBS Passive Solar Test Facility is located in Gaithersburg, MD, (latitude 39°N, longitude 77.3°W) on an open field with no shading from the surroundings. The building is a rectangular one-story, slab on grade, frame structure, with the long axis running from east to west. The building is especially designed to be reconfigurable so that passive solar features can be installed with minimum cost and effort. For example, the interior walls are not load bearing and thus can be removed or redesigned. Also, the structure of the south ceiling could support a 0.3 m (12 in) roof pond.

A photograph showing the south elevation of the building is presented in figure 2, and the floor plane of the current configuration is shown in figure 3. The current configuration provide four cells of equal floor area and an "entry" adjoining cell #1 on the west of the building. Each cell has a floor area of 30.1 m² (324 ft²) and a total volume of 88.4 m³ (3122 ft³). A description of the cells will be given later in this section.

The building envelope or the envelope of each cell may be divided into four types of surfaces/components: ceiling/roof, floor, walls, and windows. A description of construction details and material properties for each surface type are given below.



Figure 2. Photograph of NBS Passive Solar Test Building

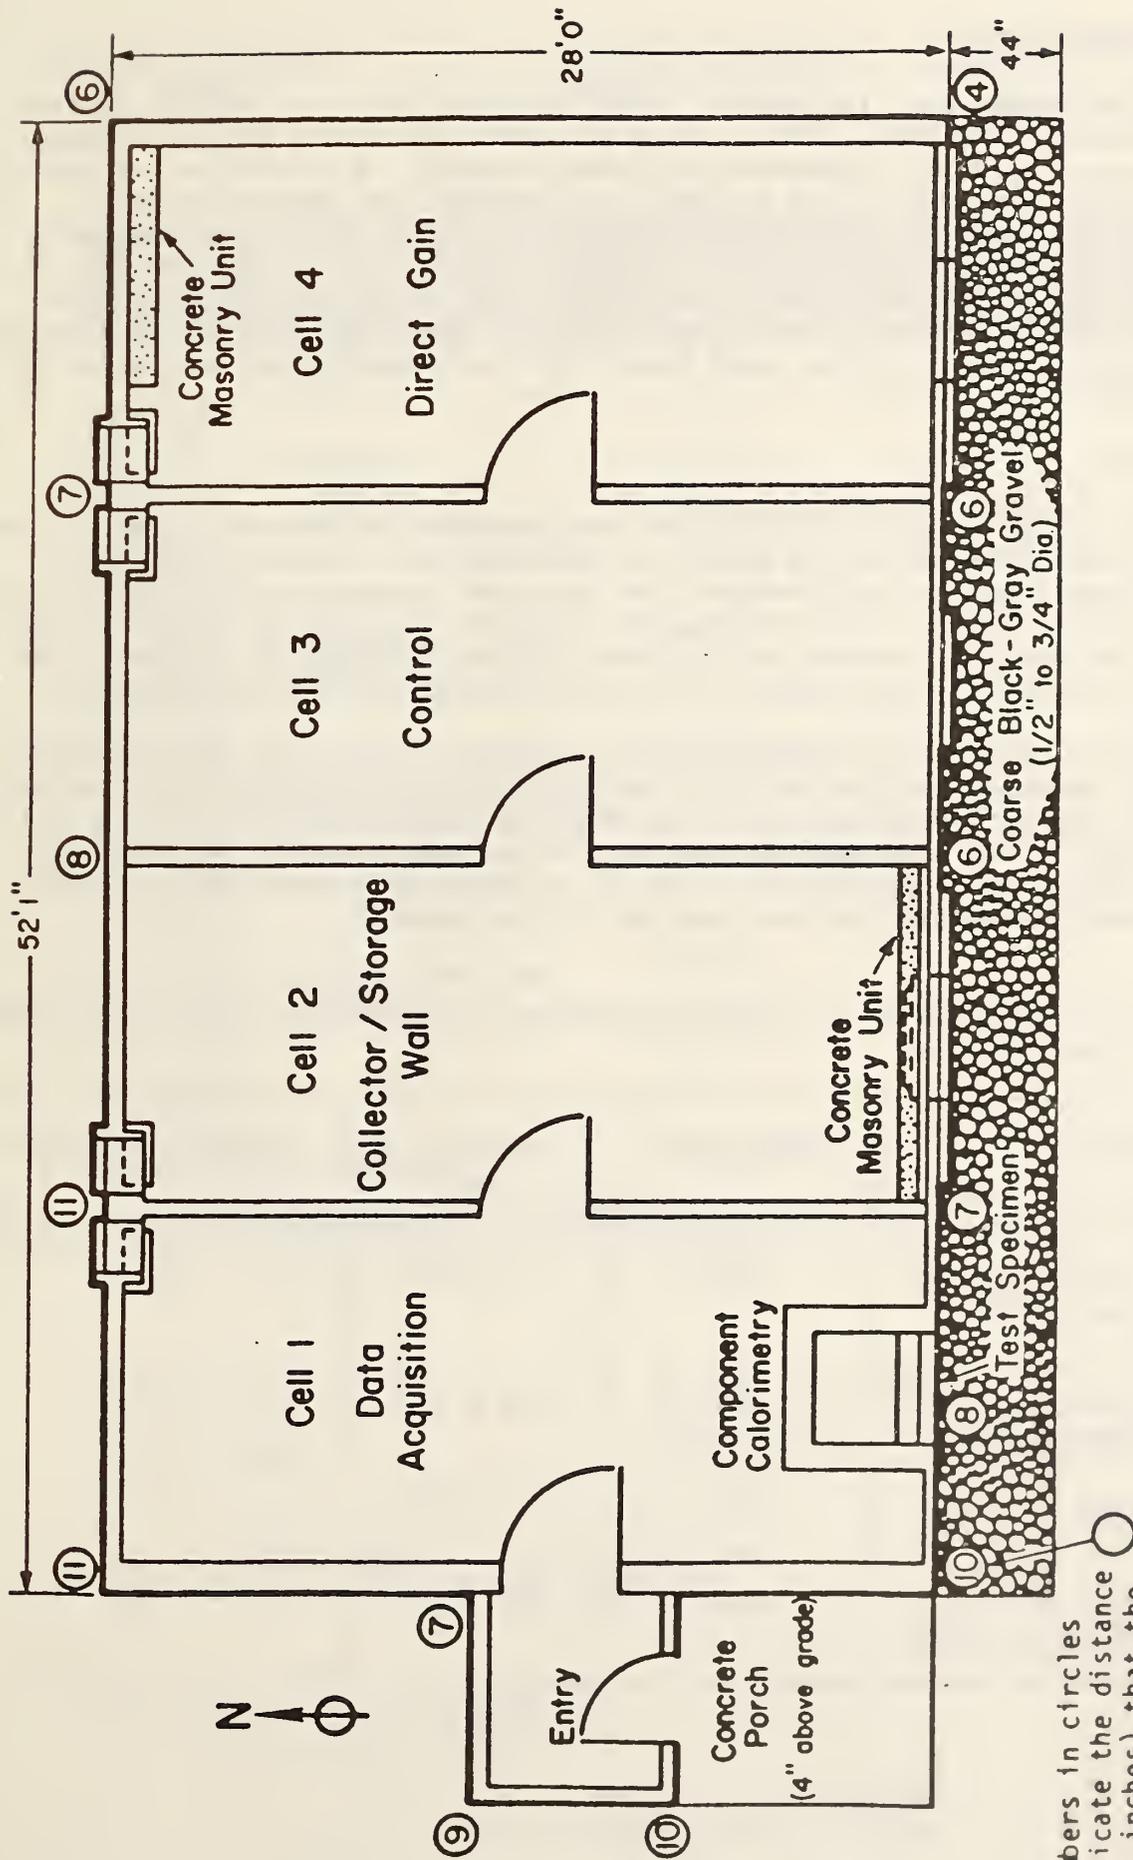


Figure 3. Floor Plan of the NBS Passive Test Building

Numbers in circles indicate the distance (in inches) that the floor surface is above the ground surface.

3.2 CEILING/ROOF

The roof is divided into two parts: a 4.77 m (15.67 ft) south section of flat builtup construction and a 4.58 m (11.25 ft) north section of asphalt shingle covered sloped roof to accommodate clerestory windows. Both sections of the roof are insulated with 240 mm (9.5 in) of fiberglass bat insulation. The ceiling height under the flat roof is 2.45 m (8.08 ft). The ceiling height under the sloped roof section varies from 4.64 m (15.25 ft) at the south end to 2.45 (8.08 ft) at the north end. A section view of both the flat and sloped roof are shown in figures 4 and 5, respectively. The properties of the construction materials as well as the total R-value of the component are also given in the figures.

3.3 FLOOR

The floor, a slab on grade construction, was designed to be of 102 mm (4 in) of concrete over 102 mm (4 in) of gravel on compacted soil. However, the core samples taken from the slab revealed that the slab thickness varies from 120 to 150 mm (4.8 to 6.0 in). The core samples also indicate that the gravel beneath the slab has settled, leaving an air gap of 0.0 to 30 mm (0.0 to 1.2 in). The details of core drilling locations and slab thickness are shown in figure 6.

Most of the floor slab is constructed with concrete which is not air entrained, while the removable sections of the floor in the direct gain cell (cell #4) are built with air entrained concrete. The measured values of density and thermal conductivity of the slab material and the storage wall material are given in table 1. Floor is insulated with 50 mm (2 in) extruded polystyrene insulation board along the perimeter slab to the top of the footings.

Table 1. Measured Values of Density and Thermal Conductivity of Slab and Storage Wall Material

Material	Temperature °C	Density, ρ kg/m ³	Thermal Conductivity, k W/m°C
<u>Concrete</u> , (air-entrained removable floor section in cell #4)	22.4	2.2×10^3	1.37
<u>Concrete</u> , not air-entrained floor slab	22.6	2.3×10^3	1.45
<u>Concrete block</u> storage wall	23.8	1.5×10^3	0.56
<u>Mortar</u> , within the cores of concrete blocks	21.9	1.9×10^3	1.03


Thermal Resistance
(at framing)

Thermal Resistance
(between framing)

Heat Capacity

Surface $\alpha_s = .60$
 $\epsilon = .90$

Concrete Paver
(see Fig 6)

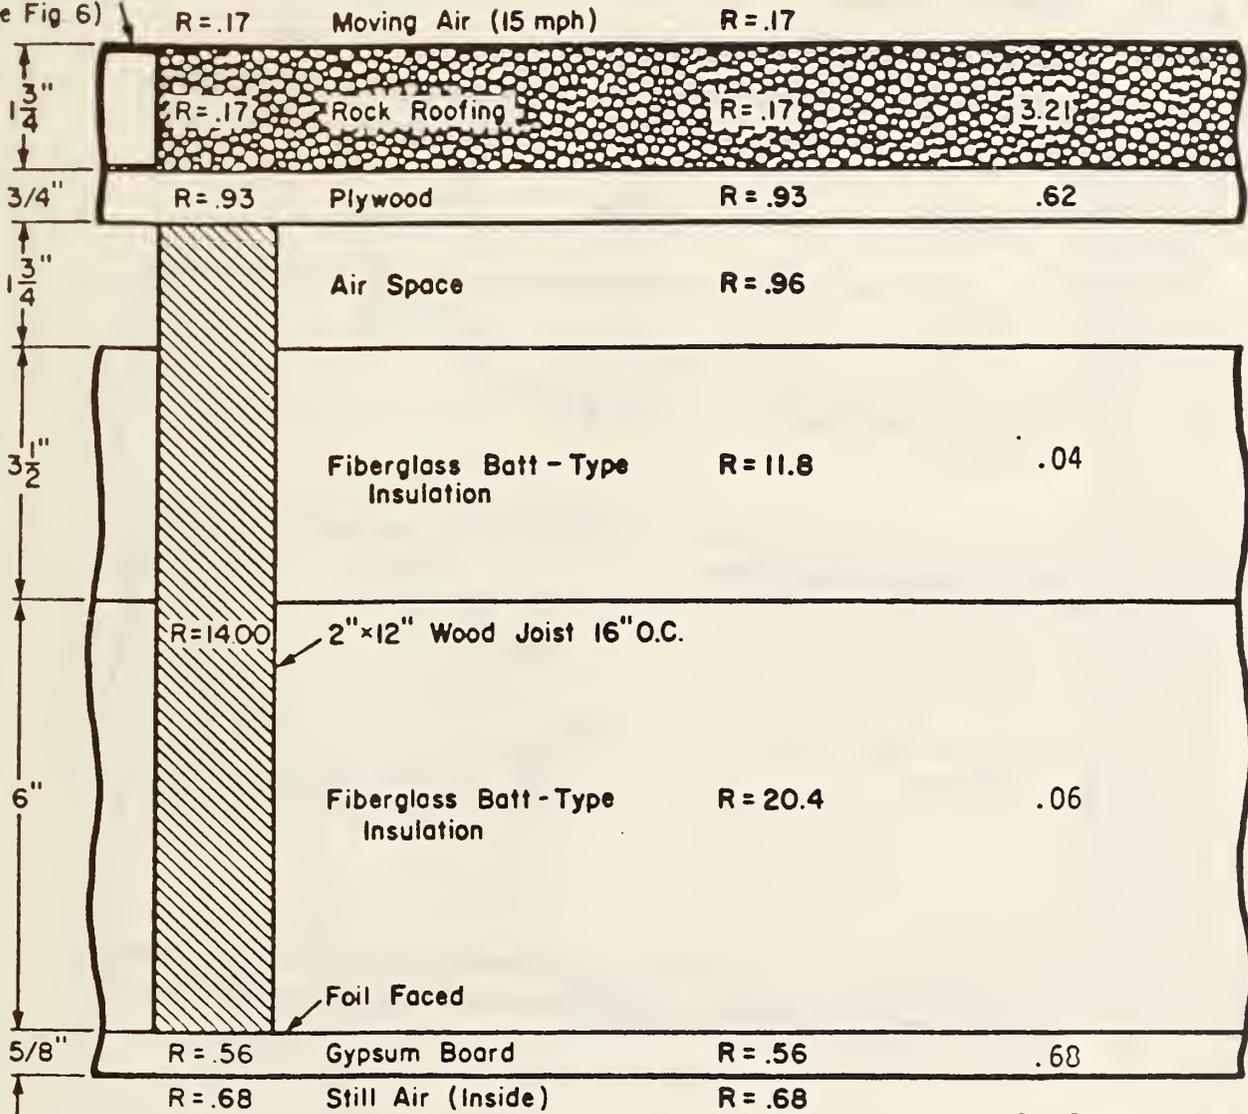

Surface = $\alpha_s = 0.23$
 $\epsilon = 0.78$

$$R_s = 16.51$$

$$\text{Area} = 9.5\%$$

$$R_i = 35.37$$

$$\text{Area} = 90.5\%$$

$$\frac{mC_p}{A} = \frac{4.61 \text{ Btu/ft}^2 \cdot \text{°F}}{94.2 \text{ KJ/m}^2 \cdot \text{°C}}$$


$$U_{AV} = \frac{.095}{16.51} + \frac{.905}{35.67} = .0312 \text{ Btu/ft}^2 \cdot \text{hr} \cdot \text{°F}$$

$$(.177 \text{ W/m}^2 \cdot \text{°C})$$

$$R_{AV} = \frac{1}{U_{AV}} = 32.05 \text{ ft}^2 \cdot \text{hr} \cdot \text{°F/Btu}$$

$$(5.644 \text{ m}^2 \cdot \text{°C/W})$$

Figure 4. Cross Section of the Flat Roof

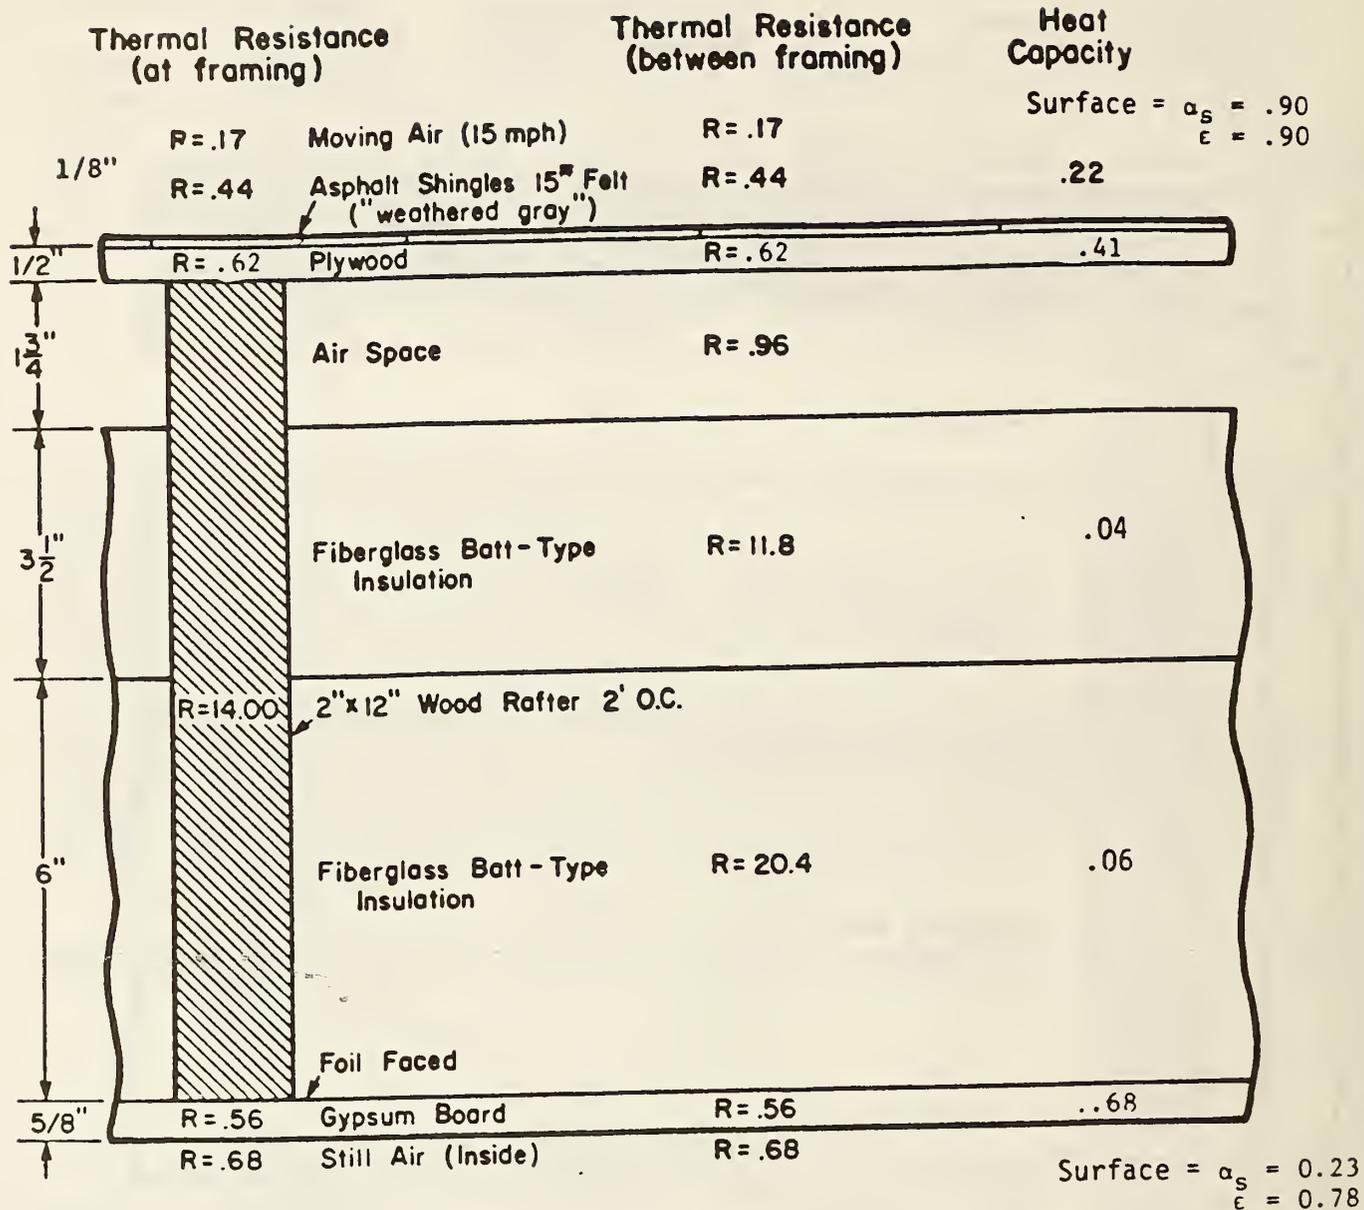

$$R_s = 16.47$$

$$\text{Area} = 6.5\%$$

$$R_i = 35.63$$

$$\text{Area} = 93.5\%$$

$$\frac{mC_p}{A} = 1.41 \text{ Btu/ft}^2\text{°F}$$

$$(28.8 \text{ KJ/m}^2\text{°C})$$


$$U_{AV} = \frac{.065}{16.47} + \frac{.935}{35.64} = .0301 \text{ Btu/ft}^2\text{hr°F}$$

$$(.1716 \text{ W/m}^2\text{°C})$$

$$R_{AV} = \frac{1}{U_{AV}} = 33.22 \text{ ft}^2\text{hr°F/Btu}$$

$$(5.350 \text{ m}^2\text{°C/W})$$

Figure 5. Cross Section of the Sloped Roof

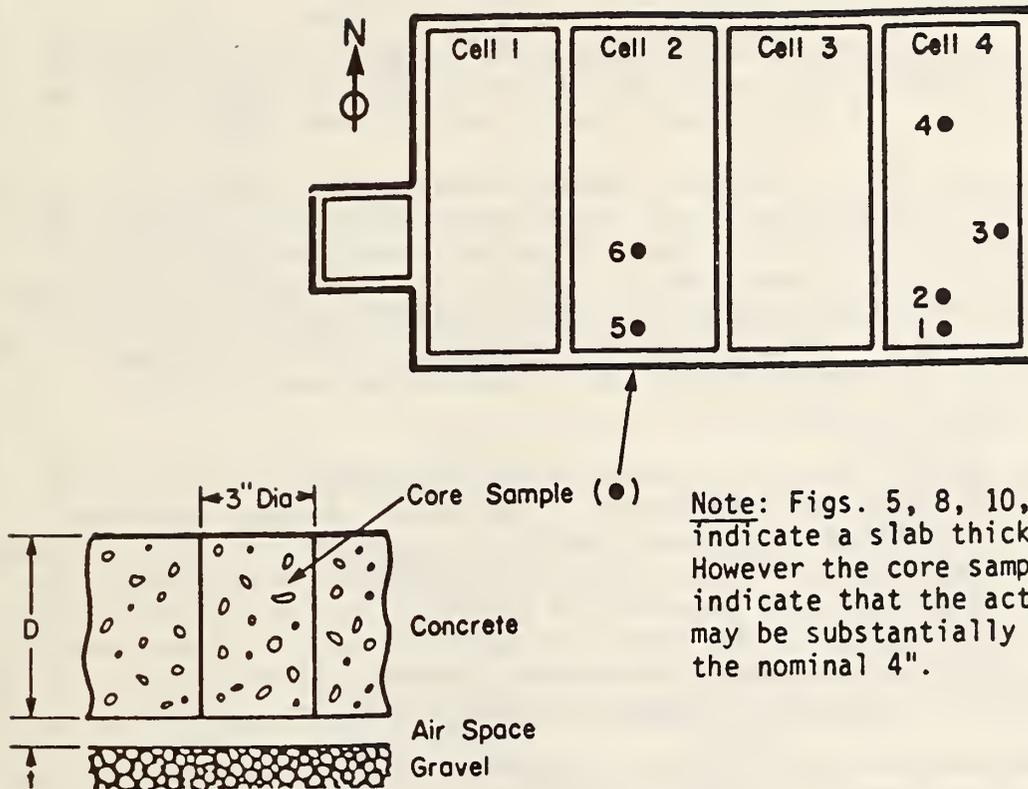

Note: Figs. 5, 8, 10, 12, and 14 indicate a slab thickness of 4". However the core samples taken indicate that the actual thickness may be substantially different than the nominal 4".

Core No.	Distance from South Wall of Cell	Distance from East Wall of Cell	Core Thickness D (in)	Air Space t (in)
1	1' 2"	6' 0"	5.6	0.1
2	2' 7"	6' 1"	6.0	0.0
3	10' 8"	1' 0"	4.9	0.8
4	17' 11"	6' 0"	5.1	0.1
5	1' 3"	6' 0"	5.7	0.1
6	9' 9"	6' 2"	4.8	1.2

Figure 6. Core Drilling Locations and Slab Thicknesses

3.4 WALLS

The walls may be divided into the following five types: (1) east and west outer walls; (2) inner partition walls; (3) north wall; (4) south wall; and (5) thermal storage wall. A description of each type is given below.


East and West Outer Walls. The east and west outside walls are double-stud (two rows of 2 x 4's separated by air space) frame construction covered with insulating sheathing and cedar siding. These walls are insulated with two layers of 90 mm (3.5 in) fiberglass batt insulation. The double studing and extra insulation are used to reduce the heat transfer through the end walls. A section view showing the construction of these walls is shown in figure 7. The properties of the construction materials as well as the total R-value of the wall are also given in figure 7.

Inner Partition Walls. The inner partition walls, separating the adjacent cells, are single-stud frame construction. Both sides of these walls have 38 mm (1.5 in) of extruded polystyrene behind the gypsum board, and are insulated with 90 mm (3.5 in) fiberglass batt insulation. A section view showing the construction of these walls is presented in figure 8. The properties of the materials of construction and the total R-value of the wall are also shown in figure 8. Heavily insulated metal doors with a thermal resistance of $0.44 \text{ m}^2\text{C/W}$ ($R=2.5$) serve as a passageway between the cells.

North Wall. The north outside wall is single-stud frame construction covered with insulating sheathing and cedar siding. The wall is insulated with 90 mm (3.5 in) fiberglass batt insulation. The section view, showing the construction details, material properties, and total R-value of the wall is given in figure 9. The north wall contains a wood casement window for each cell. A plane and section view of the north wall, shown in figure 10, indicates the location of the window and the fan coil unit.

South wall. The south wall is divided into two levels: upper south wall and lower south wall. The upper south wall contains a clerestory window for each cell. The opaque portions of the upper level south wall are of single-stud frame construction covered with 12.7 mm (0.5 in) plywood and cedar siding and insulated with 90 mm (3.5 in) fiberglass batt insulation. Figure 11 shows a section view of the opaque portion of the upper south wall along with the material properties and total R-value for the wall.

The lower level south wall in each cell is different to accommodate different passive solar features. The opaque portion of the lower south wall is of the same construction as the north wall described previously.

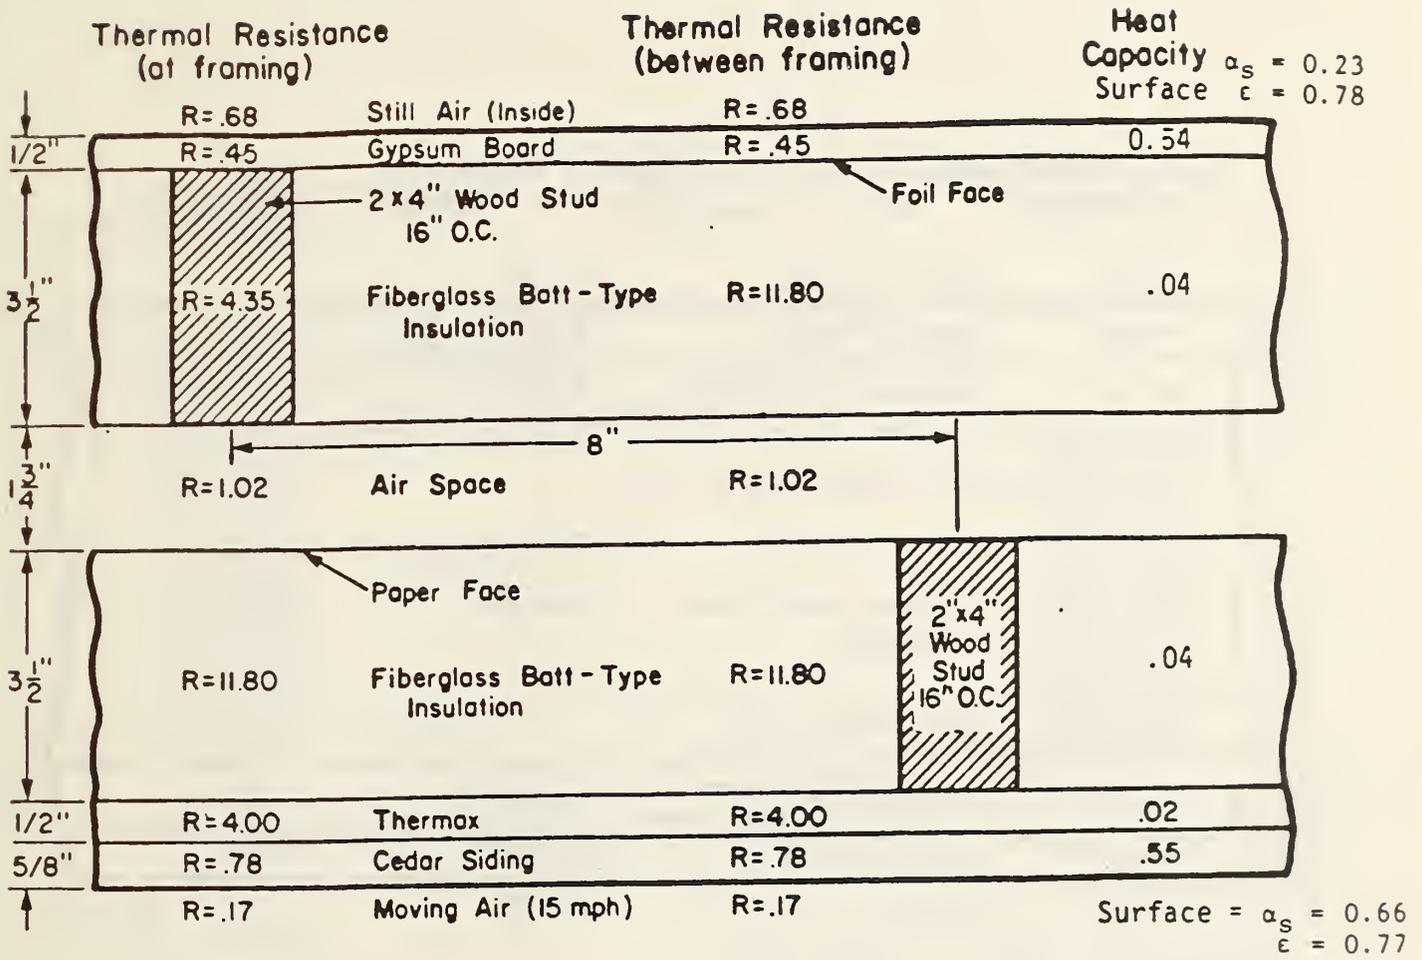

$$R_s = 23.25$$

$$\text{Area} = 30\%$$

$$R_i = 30.6$$

$$\text{Area} = 70\%$$

$$\frac{mCp}{A} = 1.19 \text{ Btu/ft}^2 \text{ } ^\circ\text{F}$$

$$(24.3 \text{ KJ/m}^2 \text{ } ^\circ\text{C})$$

$$U_{AV} = \frac{.3}{23.25} + \frac{.7}{30.6} = .03570 \text{ Btu/ft}^2 \text{hr}^\circ\text{F}$$


$$(.2027 \text{ W/m}^2 \text{ } ^\circ\text{C})$$

$$R_{AV} = 28.01 \text{ ft}^2 \text{hr}^\circ\text{F/Btu}$$

$$(4.932 \text{ m}^2 \text{ } ^\circ\text{C/W})$$

Note: Although the studs are 8" from center to center (accounting for the double wall) in calculating R values they are assumed to occupy 30% of the wall area in order to compensate for multi-directional heat flow and because of the additional studs used in corners and as top and bottom plates.

Figure 7. Cross Section of the East/West Outside Walls

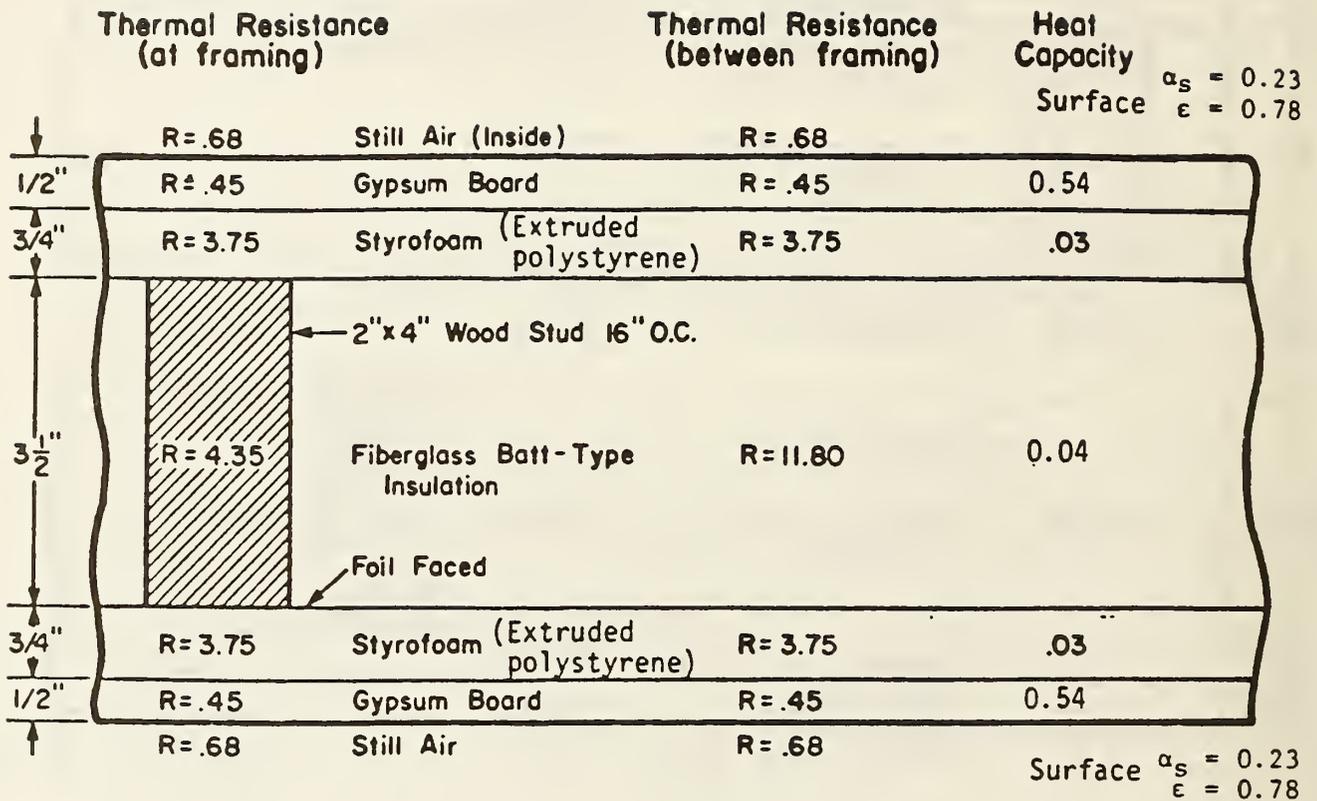

$$R_s = 14.11$$

$$\text{Area} = 20\%$$

$$R_i = 21.56$$

$$\text{Area} = 80\%$$

$$\frac{mCp}{A} = 1.18 \text{ Btu/ft}^2 \text{ } ^\circ\text{F}$$

$$(24.2 \text{ KJ/m}^2 \text{ } ^\circ\text{C})$$

$$U_{AV} = \frac{.2}{14.11} + \frac{.8}{21.56} = .05128 \text{ Btu/ft}^2 \text{ hr}^\circ\text{F}$$


$$(.2910 \text{ W/m}^2 \text{ } ^\circ\text{C})$$

$$R_{AV} = \frac{1}{U_{AV}} = 19.50 \text{ ft}^2 \text{ hr}^\circ\text{F/Btu}$$

$$(3.434 \text{ m}^2 \text{ } ^\circ\text{C/W})$$

Note: Although the studs are 16" from center to center, in calculating R values, they are assumed to occupy 20% of the wall area in order to compensate for multidirectional heat flow and because of the additional studs used around doors, in corners, and as top and bottom plates.

Figure 8. Cross Section of the Inside Partition Wall

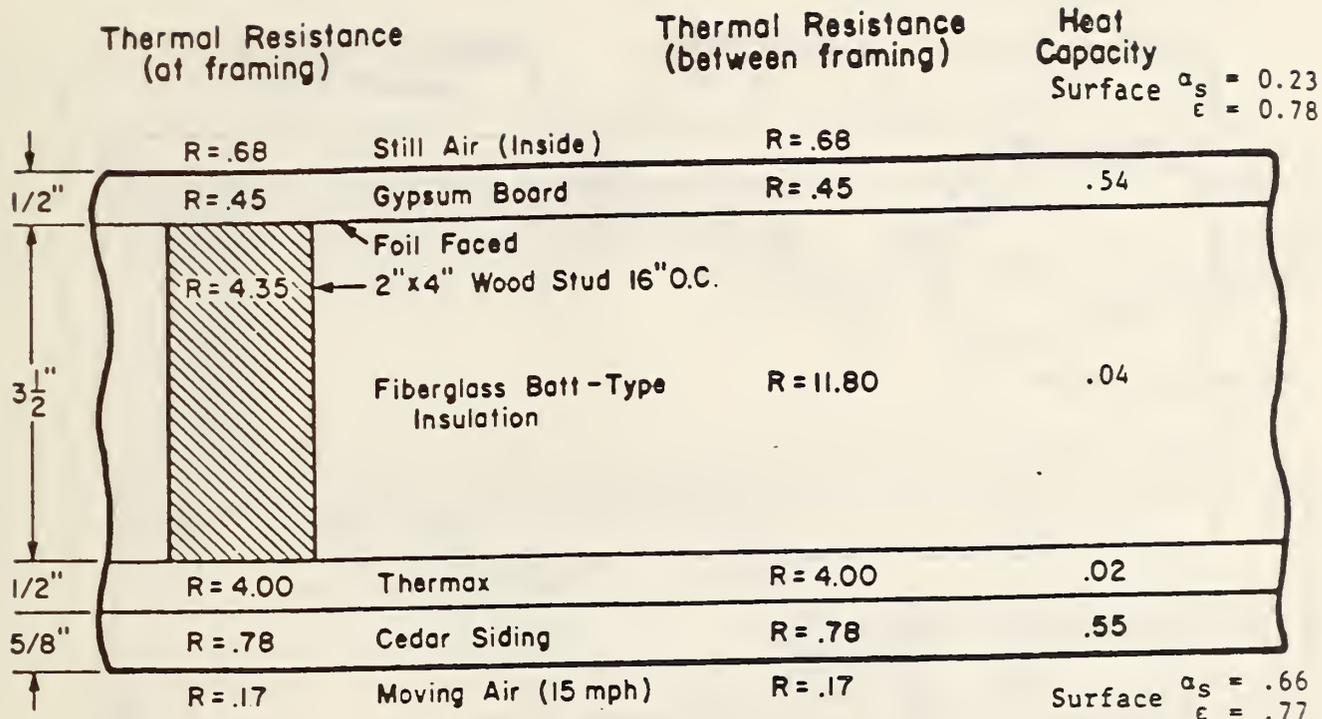

$$R_s = 10.43$$

Area = 20%

$$R_i = 17.88$$

Area = 80%

$$\frac{mC_p}{A} = 1.15 \text{ Btu/ft}^2 \cdot \text{°F}$$

$$(\rho 3.5 \text{ KJ/m}^2 \cdot \text{°C})$$

$$U_{AV} = \frac{.2}{10.43} + \frac{.8}{17.88} = .06392 \text{ Btu/ft}^2 \cdot \text{hr} \cdot \text{°F}$$

$$(.3629 \text{ W/m}^2 \cdot \text{°C})$$

$$R_{AV} = \frac{1}{U_{AV}} = 15.65 \text{ ft}^2 \cdot \text{hr} \cdot \text{°F/Btu}$$

$$(2.755 \text{ m}^2 \cdot \text{°C/W})$$

Figure 9. Cross Section of the North Wall


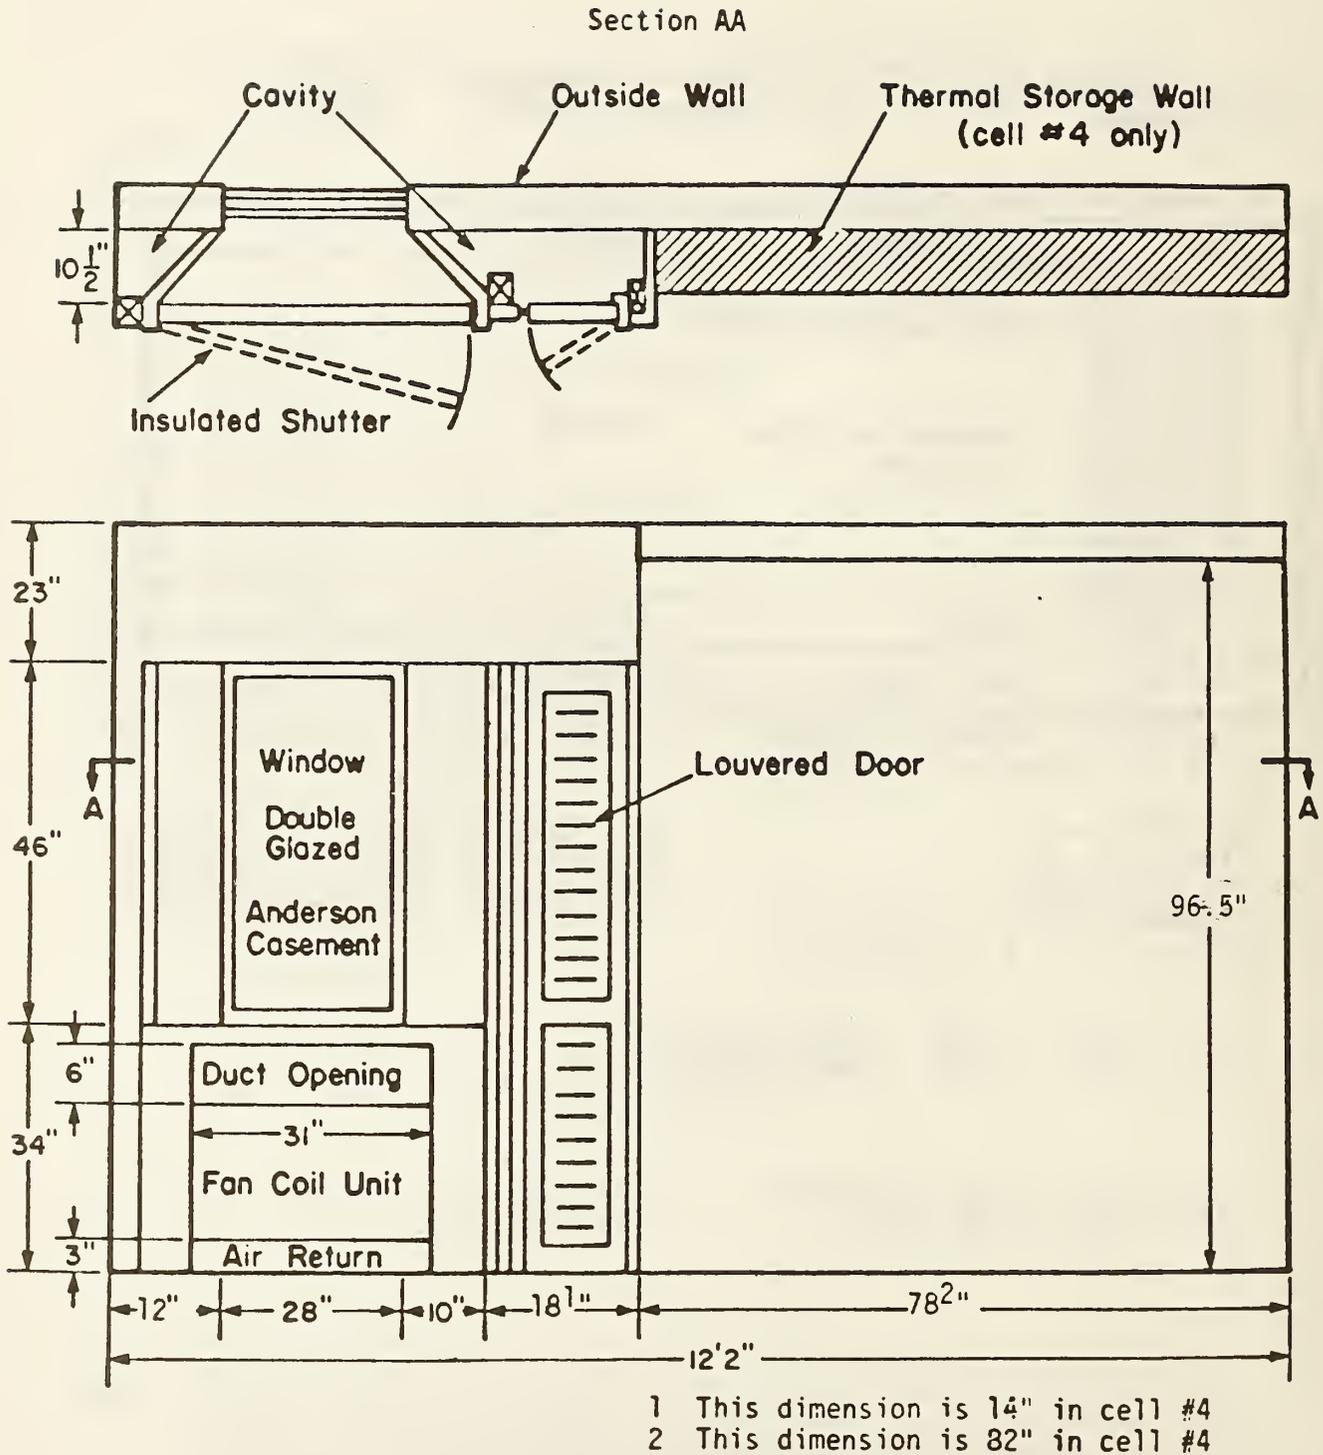


Figure 10. Plan and Section View of the North Wall
(Cell #1 and #3 are reversed)

Thermal Resistance
(at framing)

Thermal Resistance
(between framing)

Heat Capacity
Surface $\alpha_s = 0.23$
 $\epsilon = 0.78$

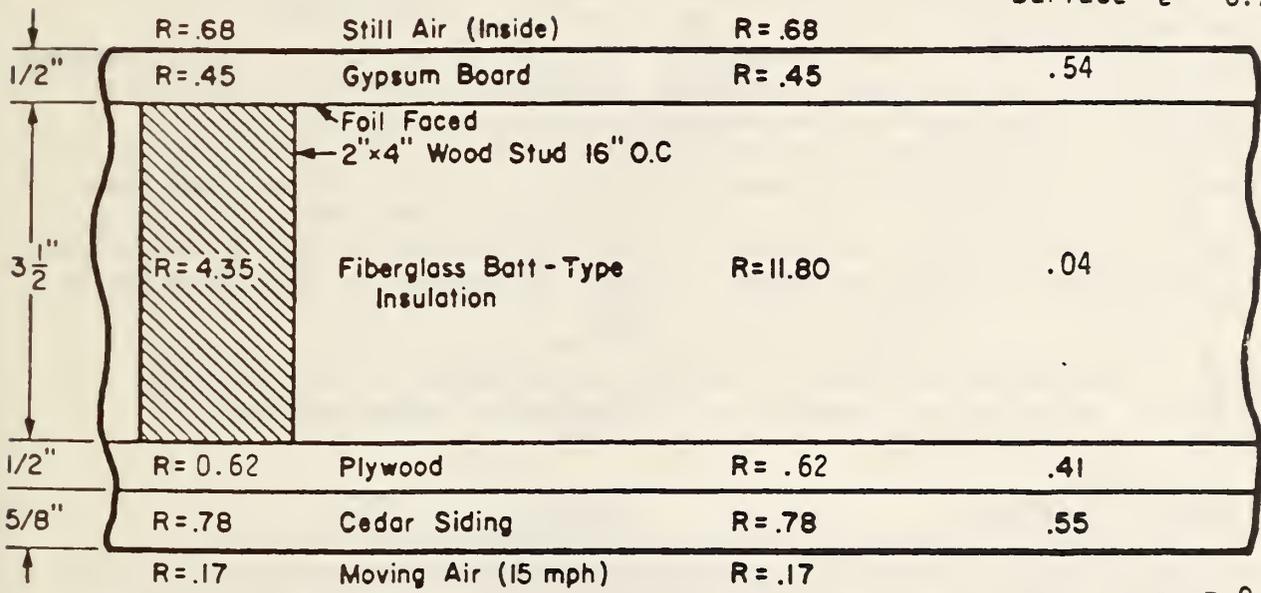

Surface $\alpha_s = 0.66$
 $\epsilon = 0.77$

$$R_s = 7.05$$

$$\text{Area} = 20\%$$

$$R_i = 14.50$$

$$\text{Area} = 80\%$$

$$\frac{mC_p}{A} = 1.54 \text{ Btu/ft}^2 \text{ } ^\circ\text{F}$$

$$(31.5 \text{ KJ/m}^2 \text{ } ^\circ\text{C})$$

$$U_{AV} = \frac{.2}{7.05} + \frac{.8}{14.50} = .0836 \text{ Btu/ft}^2 \text{hr}^\circ\text{F}$$

$$(.475 \text{ W/m}^2 \text{ } ^\circ\text{C})$$

$$R_{AV} = \frac{1}{U_{AV}} = 11.96 \text{ ft}^2 \text{hr}^\circ\text{F/Btu}$$

$$(2.110 \text{ m}^2 \text{ } ^\circ\text{C/W})$$

Figure 11. Cross Section of the Opaque Portion of Upper South Wall

3.5 WINDOWS

Each cell has a double-pane, wood casement window with an unobstructed glass area of 0.67 m^2 (7.2 ft^2) located on the north wall of each cell, and a clerestory window located on the upper level south wall. The clerestory window consists of a three-section, double-pane, wood awning window which spans the entire width of the cell with an unobstructed glass area of 3.65 m^2 (39.25 ft^2). Both the clerestory window and the north window are provided with manually operable interior insulating shutters with a thermal resistance value of $1.23 \text{ m}^2\text{C/W}$ ($R=7$). The windows in the lower south wall for each cell will be described later in section 3.8. The construction details of the headers above the windows and door are shown in figure 12 along with the properties of the materials.

A total of nine different types of windows are installed in the building. Description, location, and properties of the glass of these windows are summarized in figure 13.

3.6 INDIVIDUAL CELLS

As indicated earlier, the current configuration of the test building provided four cells of equal floor area. The surfaces and features common to all the cells have been described in section 3.1 to 3.5. The details of the special features of each cell are described below.

Cell #1 and "Entry"

A floor plan of cell #1 and "Entry" is shown in figure 14 while a longitudinal view is shown in figure 15. Access is gained to the "Entry" by a 0.91 m (3 ft) wide by 44.0 mm (1.75 in) thick solid pine door. Cell #1 is separated from the "Entry" and cell #2 by 44.0 mm (1.75 in) thick heavy metal doors (metal frame, urethane core).

The cell houses the data acquisition system, (DAS), continuous air infiltration monitoring system, power supply, and the component testing calorimeter and its DAS. A detailed description of the component testing calorimeter may be found in reference 6.

	Thermal Resistance		Heat Capacity
			Surface = $\alpha_s = 0.23$ $\epsilon = 0.78$
↓	R = .68	Still Air (Inside)	
1/2"	R = .45	Gypsum Board	.54
1 1/2"	R = 1.87	Wood	1.32
1/2"	R = .91	Air Space, T = 50 °F, ΔT = 10 °F	
1 1/2"	R = 1.87	Wood	1.32
1/2"	R = .62	Plywood	.41
5/8"	R = .78	Cedar Siding	.55
↑	R = .17	Moving Air (15 mph)	Surface = $\alpha_s = 0.66$ $\epsilon = 0.77$

$$R = 7.35$$

$$\frac{mC_p}{A} = 4.14 \text{ Btu/ft}^2\text{°F}$$

$$(84.6 \text{ KJ/m}^2\text{°C})$$

$$R = 7.35 \text{ ft}^2\text{hr}^{\circ}\text{F/Btu}$$

$$(1.294 \text{ m}^2\text{°C/W})$$

$$U = \frac{1}{R} = .136 \text{ Btu/ft}^2\text{hr}^{\circ}\text{F}$$

$$(.772 \text{ W/m}^2\text{°C})$$

Figure 12. Cross Section of the Window and Door Header

SIZE	MATERIAL	NO	JAMB SIZE	SPECIAL NAME	CODE	GLASS PROPERTIES
1	43"x43 1/2"	12	48"x48"	Anderson Permasield Awning Wind.	AP42-T	Thickness (each pane) 0.188"
2	13 1/2"x67 1/2"	1	18"x80 1/2"	1/2" Tempered Insulating Glass	M181	Distance between panes Awning & Casement windows 0.188"
3	43 1/2"x73 1/4"	1	47 1/2"x79"	1/2" Tempered Insulating Glass		Sliding glass door 0.250"
4	44 1/2"x75"	3	144 1/2"x77"	1/2" Tempered Insulating Glass		Index of refraction 1.526 [#]
5	24"x43"	2	56 1/2"x46"	Anderson Permasield Casement Wind.	Cx24T	Reflectance .15 #
6	44"x73 1/2"	3	144 1/2"x82 1/2"	Anderson Sliding Door II	T-120	Transmittance .73 #
7	45"x68 1/2"	1	45"x68 1/2"	Double Dome Clear Acrylic Skylight		
8	24"x43 1/2"	4	28"x48"	Anderson Permasield Casement Wind.	Cx14T	

+ Present test specimens (May be replaced in the future)

* On the north side of the building

Estimated properties

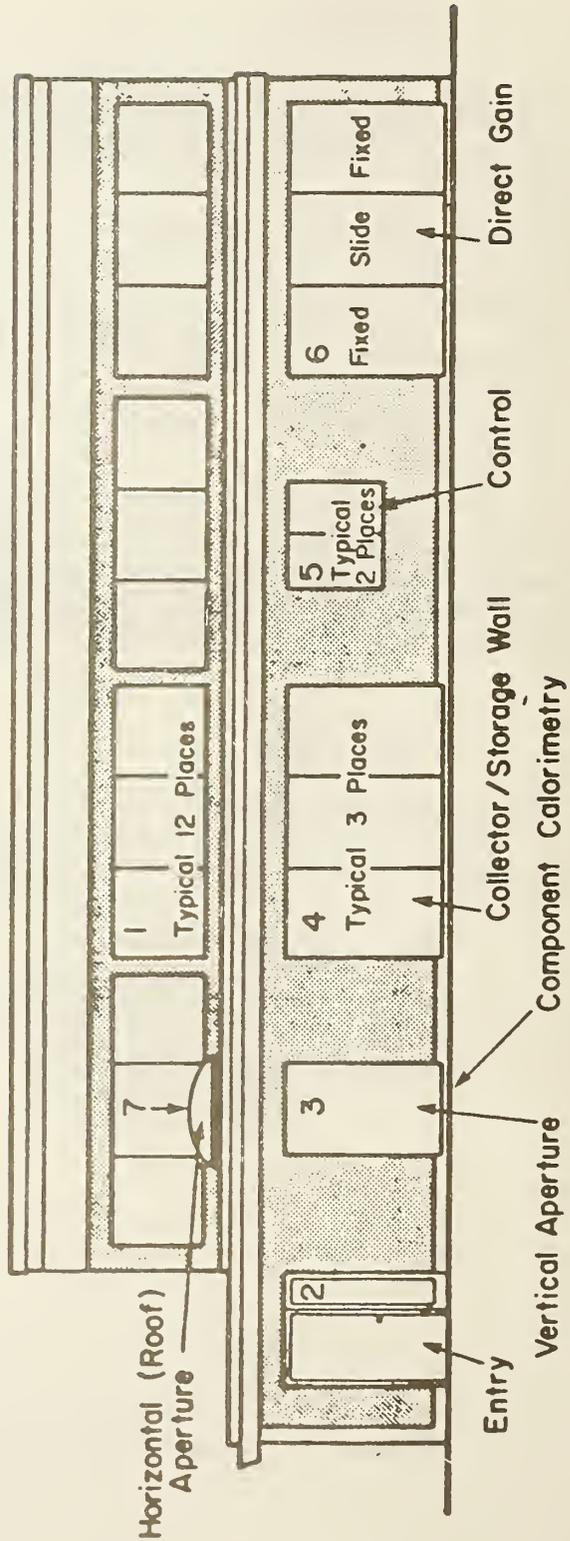


Figure 13. Window Description

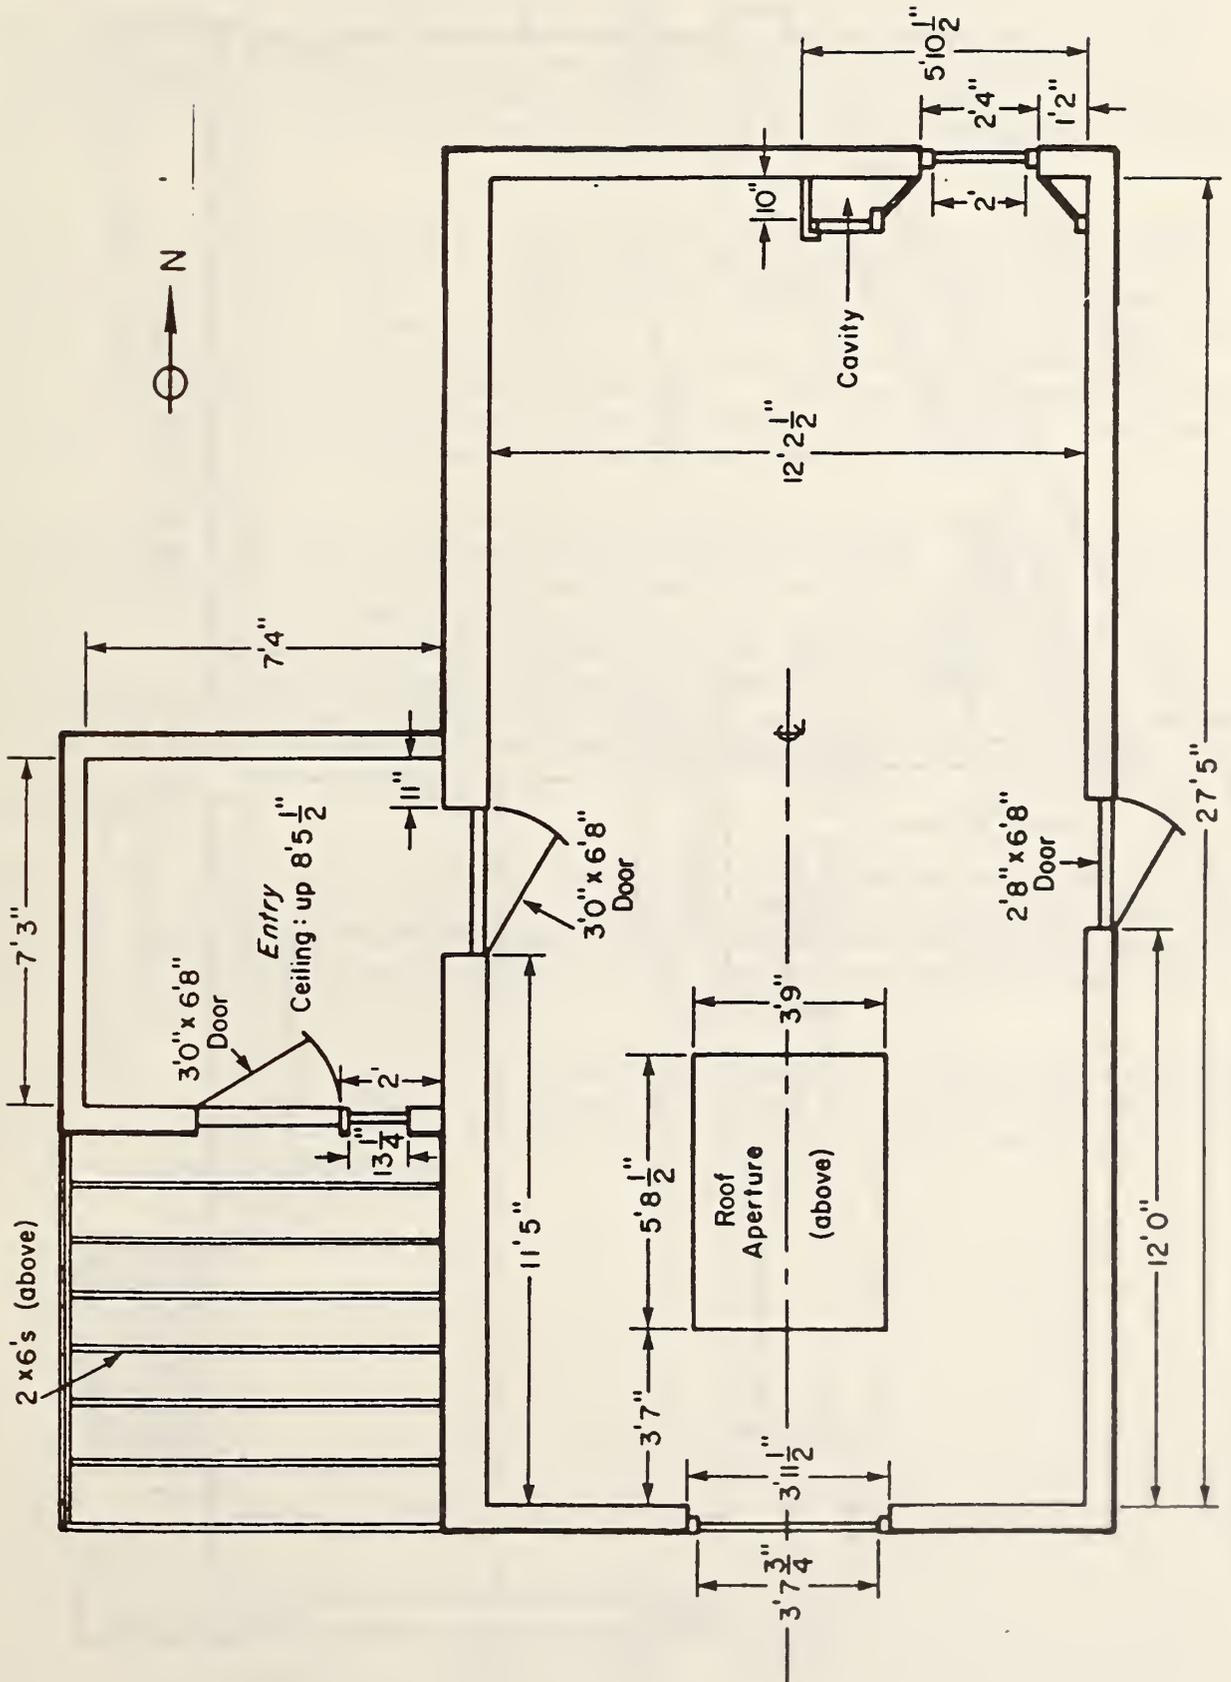


Figure 14. Floor Plan of the Component Calorimetry Cell (Cell #1)

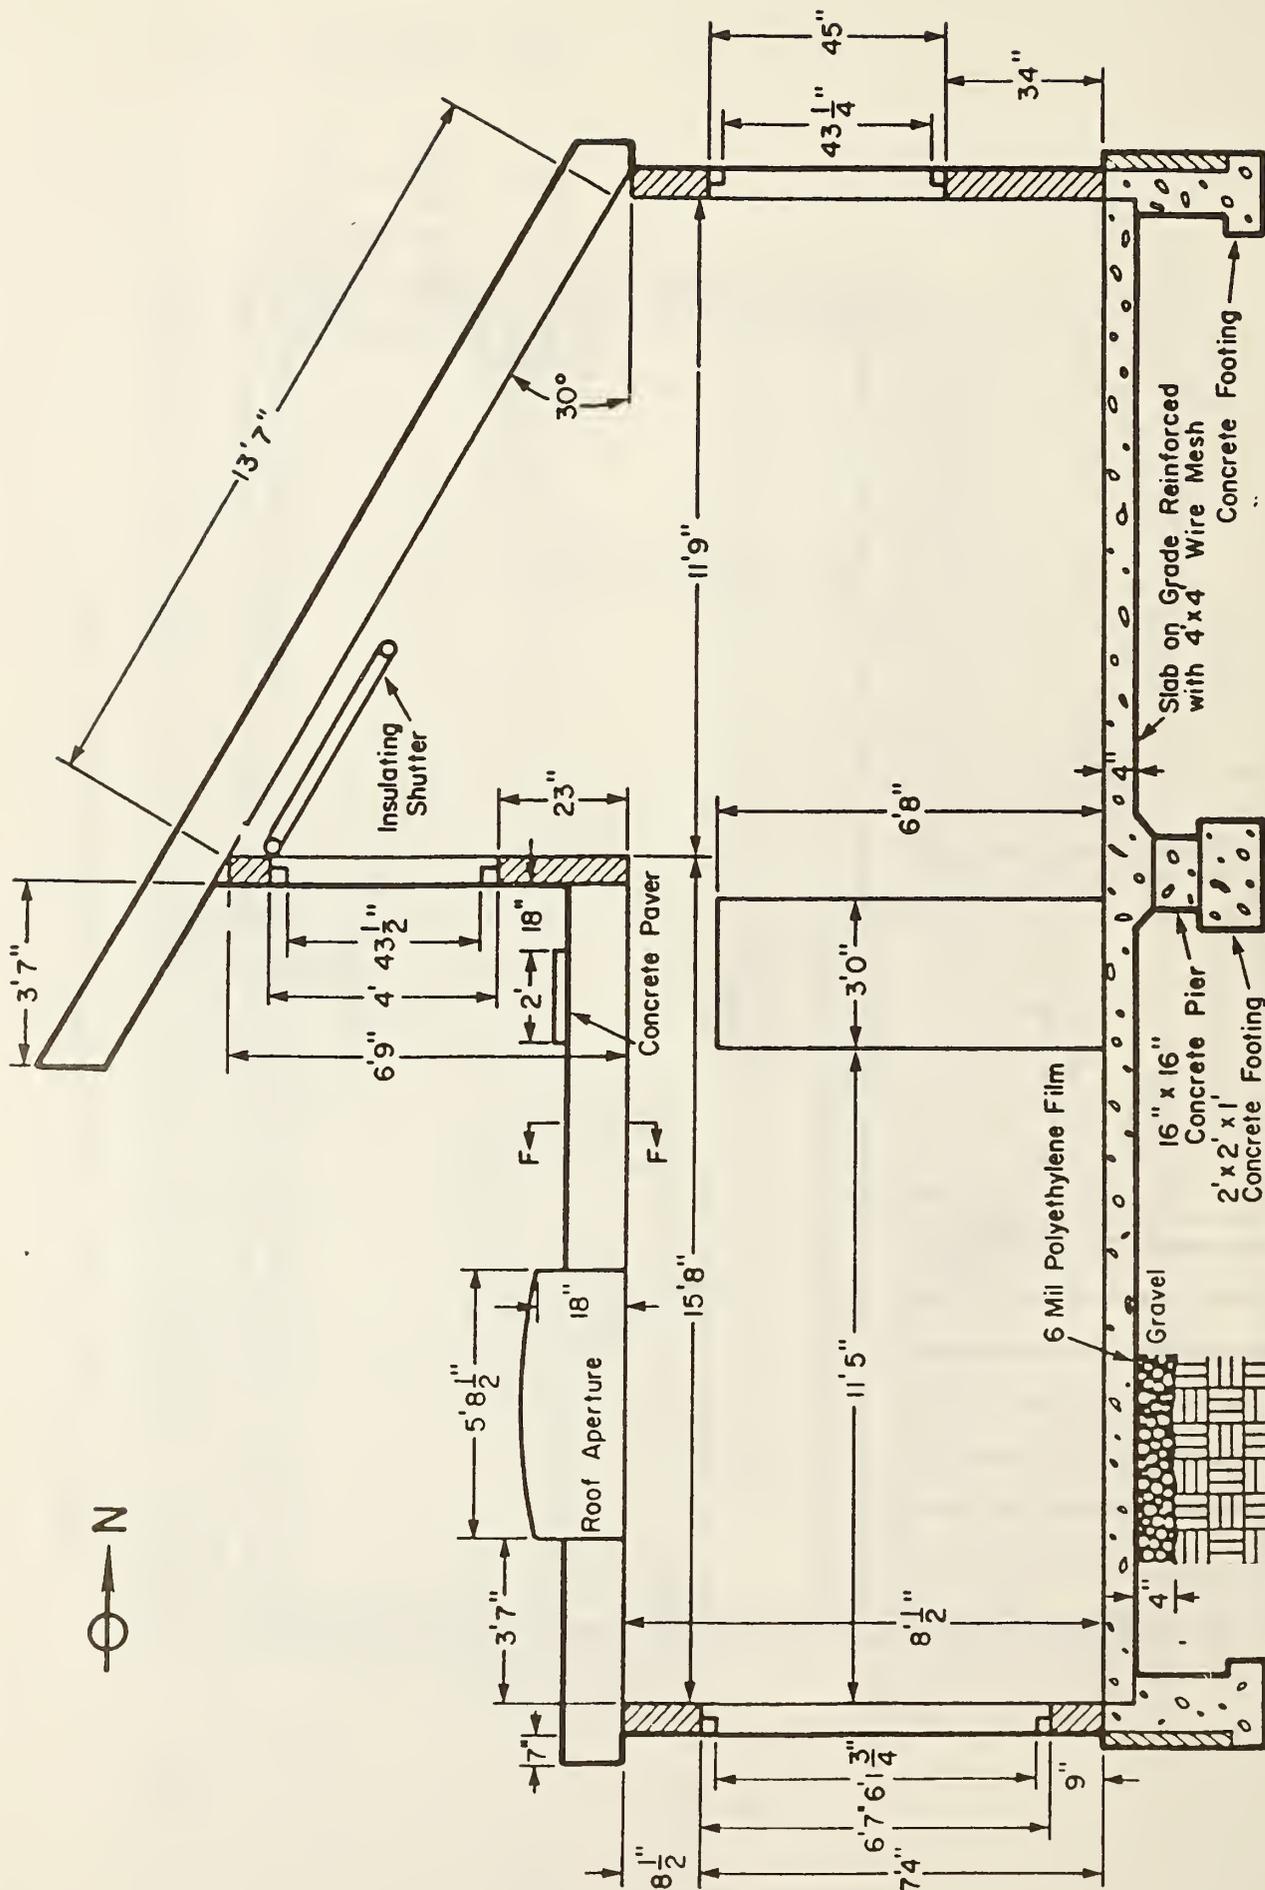


Figure 15. Longitudinal Section of the Component Calorimetry Cell

Cell #2

This is a collector storage wall cell which contains a Trombe wall over the entire width of the lower level south wall. A floor plan of the cell is given in figure 16, and a longitudinal view is shown in figure 17. Cell #2 is separated from the adjacent cells by heavy metal doors (metal frame, urethane core).

The Trombe wall is constructed of 200 x 400 x 200 mm (8 x 16 x 8 in) concrete masonry units (CMU) with cores filled with mortar. The properties of the material are given in table 1, along with the properties of concrete used for the floor slab. The Trombe wall is 3.65 m (12 ft) wide, 2.44 (8 ft) high, and 200 mm (8 in) thick. A 140 mm (5.5 in) air space separates the Trombe wall from a three-section double-glazed window wall. The glazing is made of 3.18 mm (.125 in) safety insulating glass spaced 15.9 mm (0.625 in) apart. The window dimensions and glass properties have been summarized in figure 13.

The outside surface of the Trombe wall is painted black while the inside surface is unpainted. Two vent openings, each the size of one CMU, are located 200 mm (8 in) below the top of the Trombe wall, and 609 mm (24 in) from the right and left side walls. Two identical vent openings are located 200 mm (8 in) below the top of the Trombe wall and vertically in line with the two bottom vents. A schematic of the Trombe wall is shown in figure 18. The Trombe wall can be tested in either vented or unvented conditions, and with the clerestory window shutter in either an open or closed position.

Cell #3

This is the control cell. A floor plan of the cell is shown in figure 19, and a longitudinal view is shown in figure 20. Cell #3 is separated from the adjacent cells by heavy metal doors. The purpose of the control cell is to allow for the quantitative comparison of the performances of the passive solar features in the two adjacent cells, i.e., cell #2 and cell #4.

The lower level south wall of the control cell contains a normal sized double-pane casement window. The window is 1.22 m (48 in) wide by 1.09 m (43 in) high with an unobstructed glass area of 1.34 m² (14.4 ft²). The properties of the glass are given in figure 13.

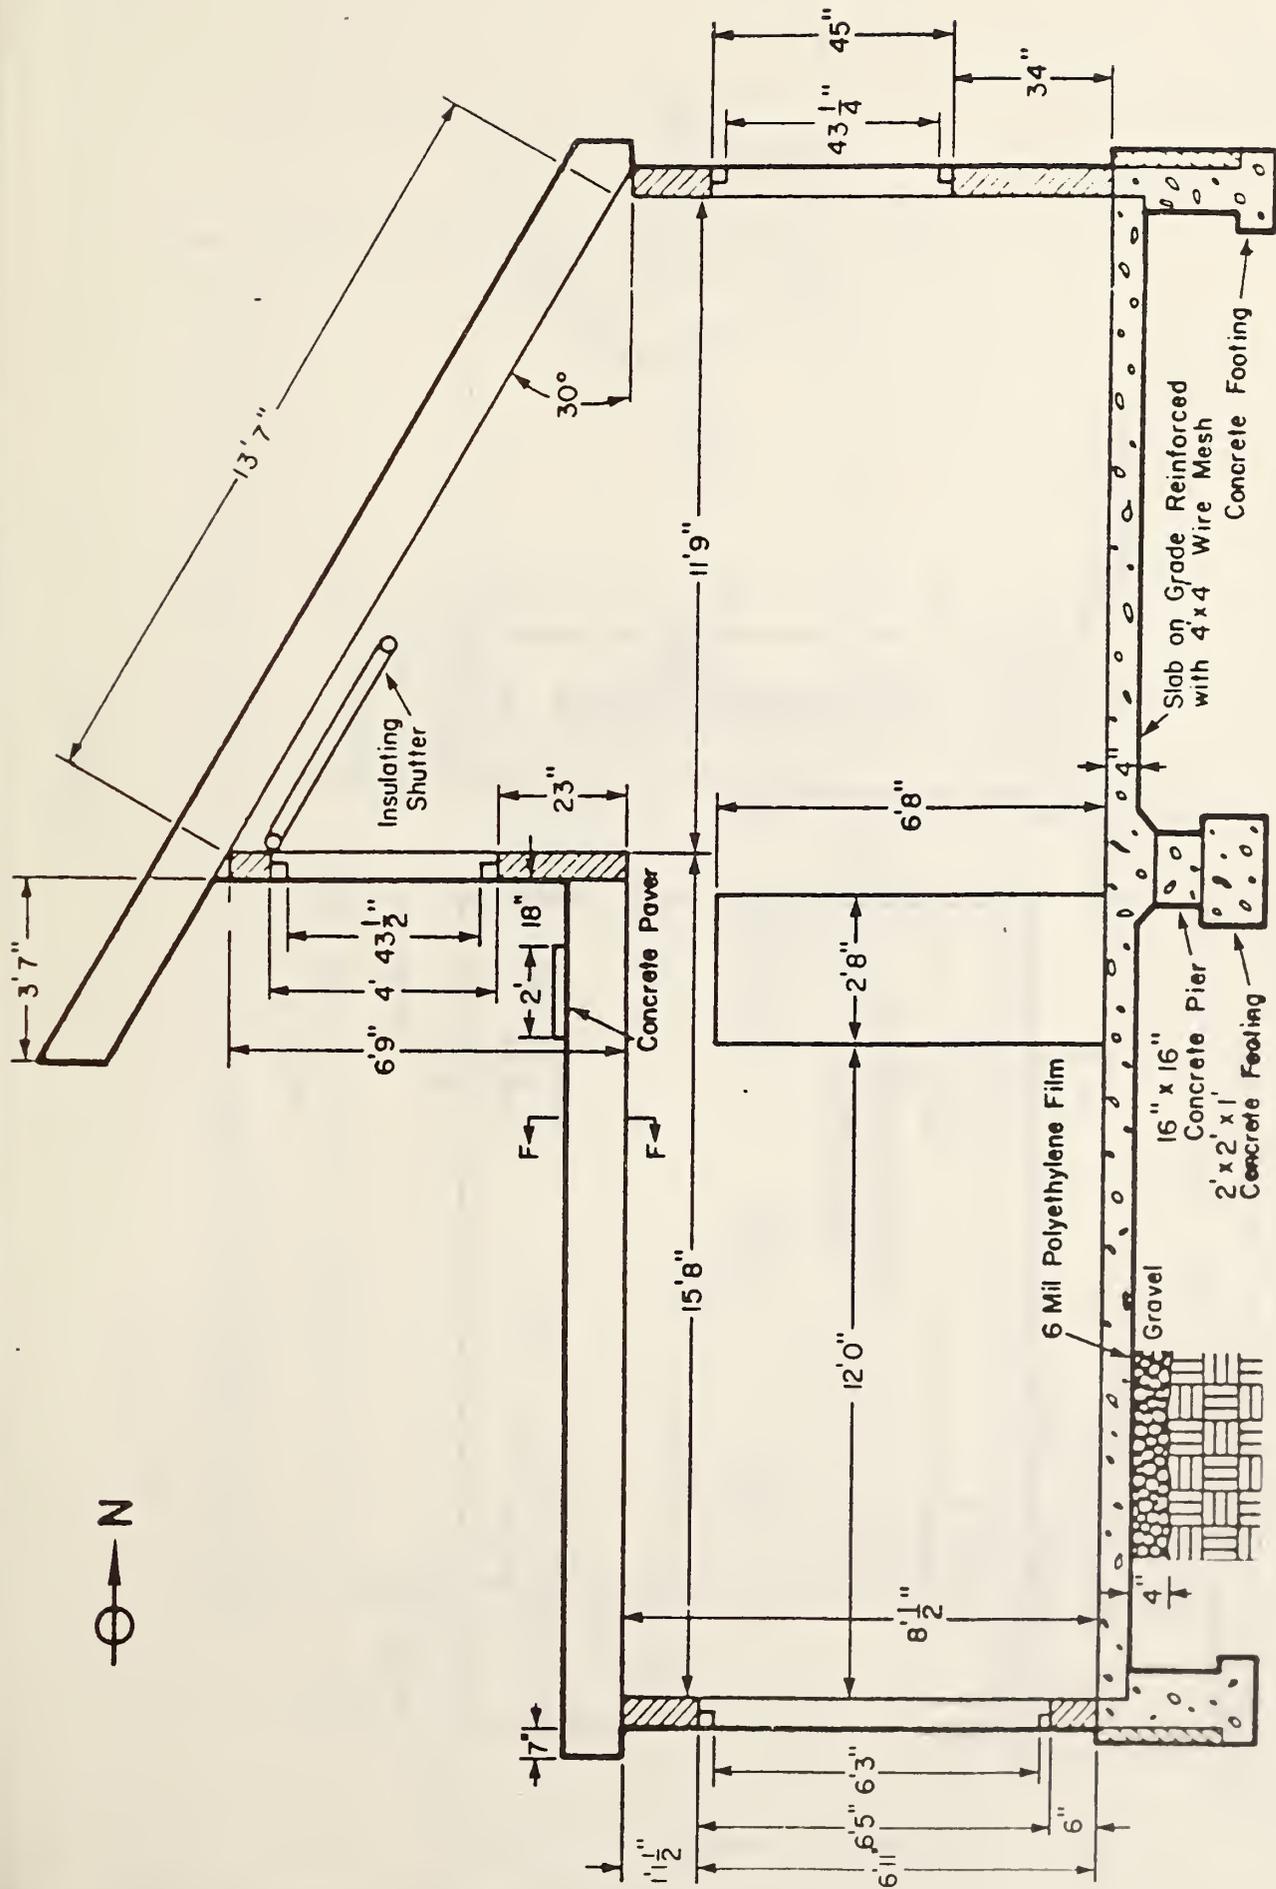


Figure 17. Longitudinal Section of the Collector/Storage Wall Cell

- * T401 T403 Inside Glazing Surface Temperature
- T404 T405 Outside Trombe Wall Surface Temperature
- T407 T409 Vent Air Temperature


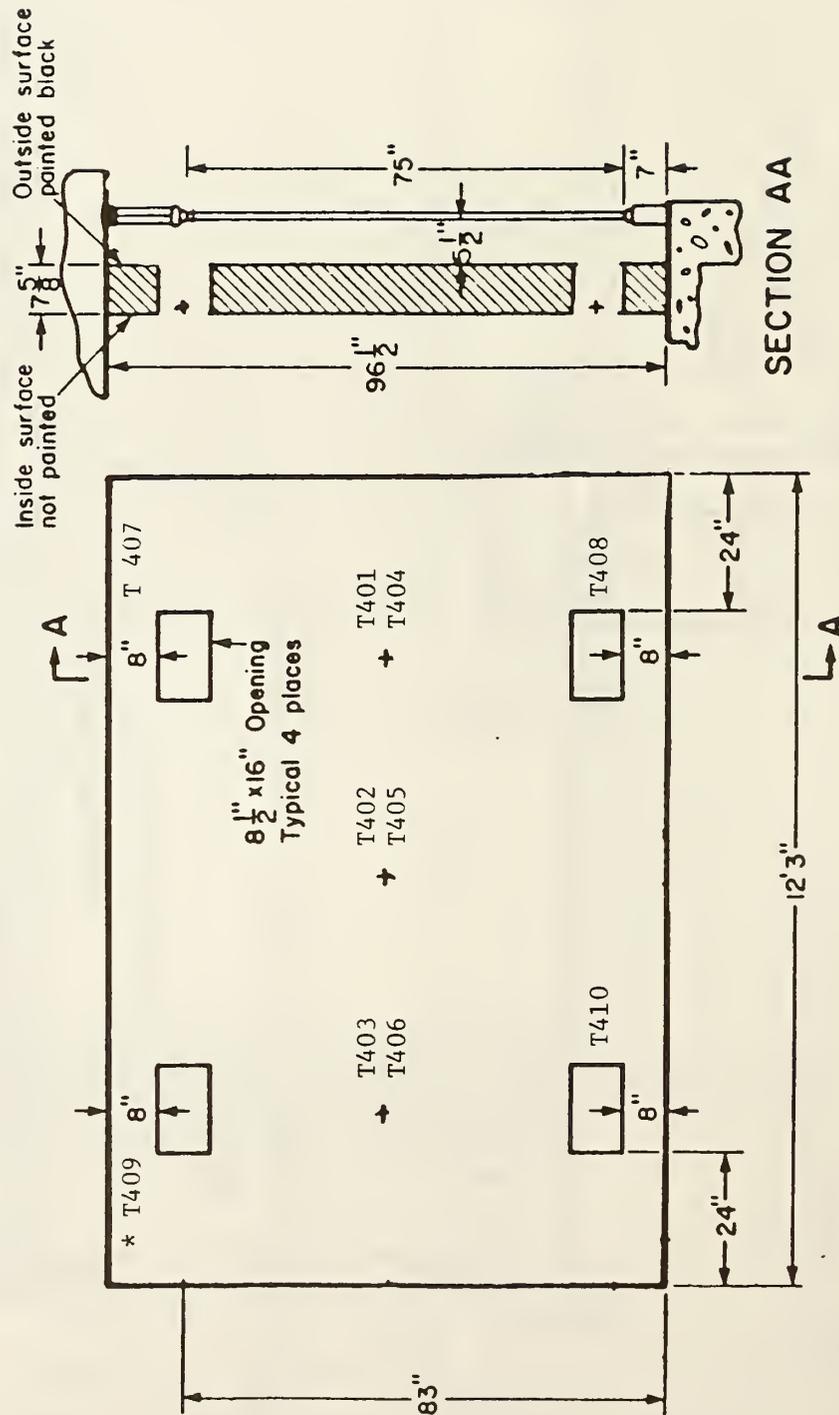


Figure 18. Schematic of the Trombe Wall

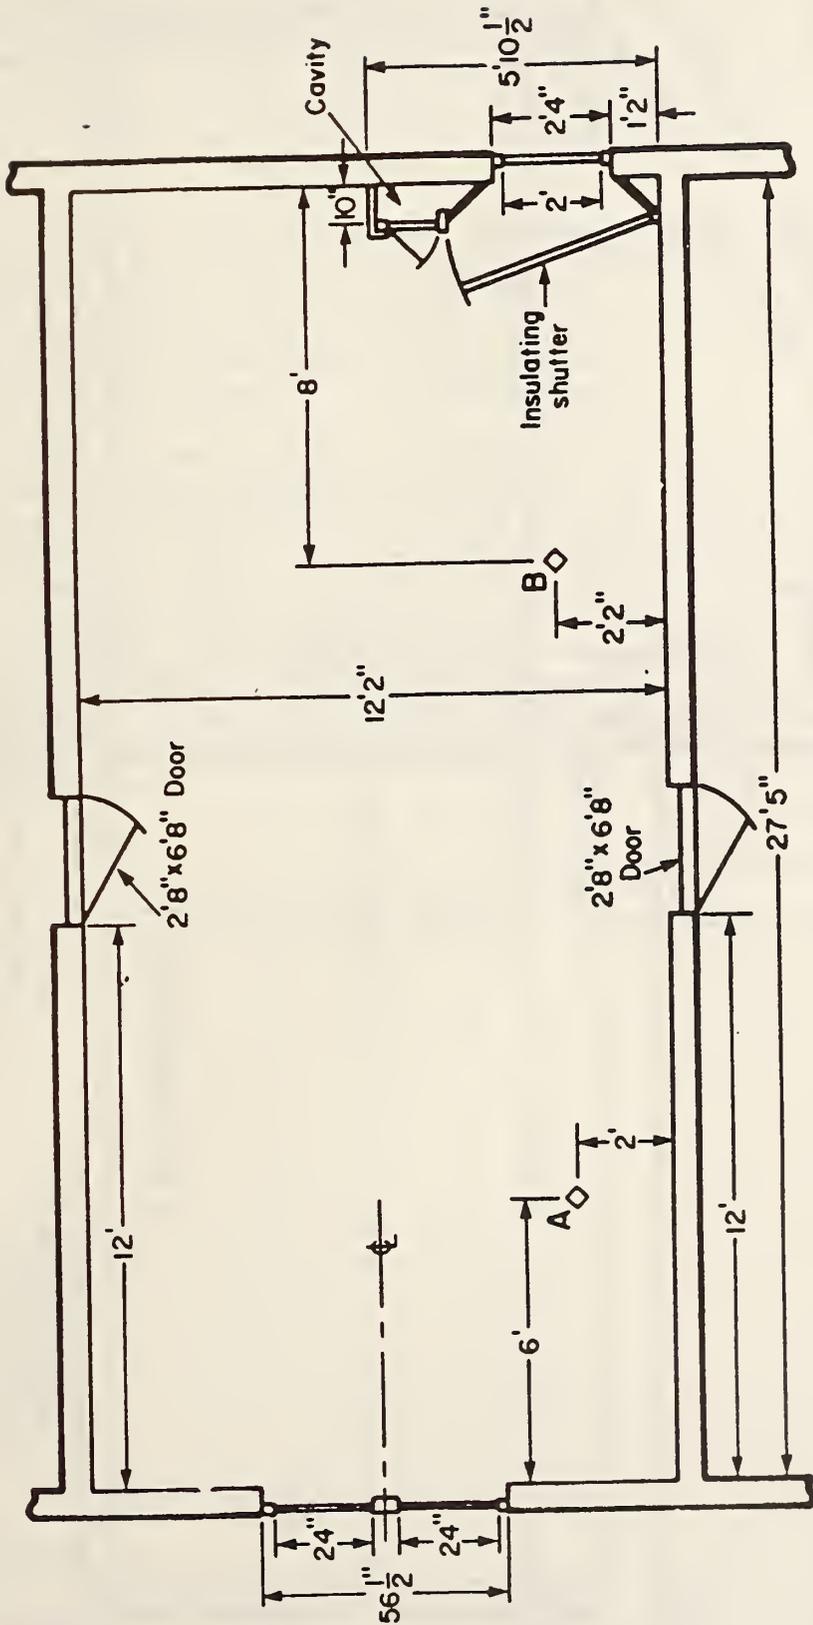

Air Temperature Thermocouples		Average of 5 T193
◇	A. 72" Above Floor	
	24" Above Floor	
	B. 20" Below Ceiling	
	74" Above Floor	
	19" Above Floor	
		T251
		T252

Figure 19. Floor Plan of the Control Cell (Cell #3)

Cell #4

This is a direct gain fenestration cell. A floor plan of the cell is shown in figure 21, and a longitudinal view is shown in figure 22. Note that there are four removable concrete floor sections bordered with paper joints. The purpose of these sections is to allow for the future addition of an underground rock storage or any other configuration modifications. Cell #4 is separated from cell #3 by a heavy metal door.

The direct gain fenestration is a double-pane wood sliding glass door covering the entire width of the lower south wall. The sliding glass door consists of two fixed sections and one sliding section. All three sections are of equal area. The total unobstructed glass area is 6.27 m² (67.53 ft²). The properties of the glass have been summarized in figure 13. As indicated earlier the upper level south wall contains a clerestory window.

Besides the thermal storage provided by the concrete floor, this cell contains additional thermal storage in the form of a 2.08 m (6.83 ft) wide by 2.46 m (8.08 ft) high by 200 mm (8 in) thick concrete masonry unit (CMU) wall located inside the north wall. The cores of the CMU's are filled with mortar, the same material as used for Trombe wall in cell #2. A section view of the thermal storage wall is shown in figure 23. The surfaces of the thermal storage wall are unpainted. A description of the direct gain cell, i.e., cell #4, is also available in reference 7. However, references 1 and 5 do not contain any information on the new data acquisition system, air infiltration monitoring system, and the sensors installed in cells #2, #3, and #4 in FY83 and FY84.

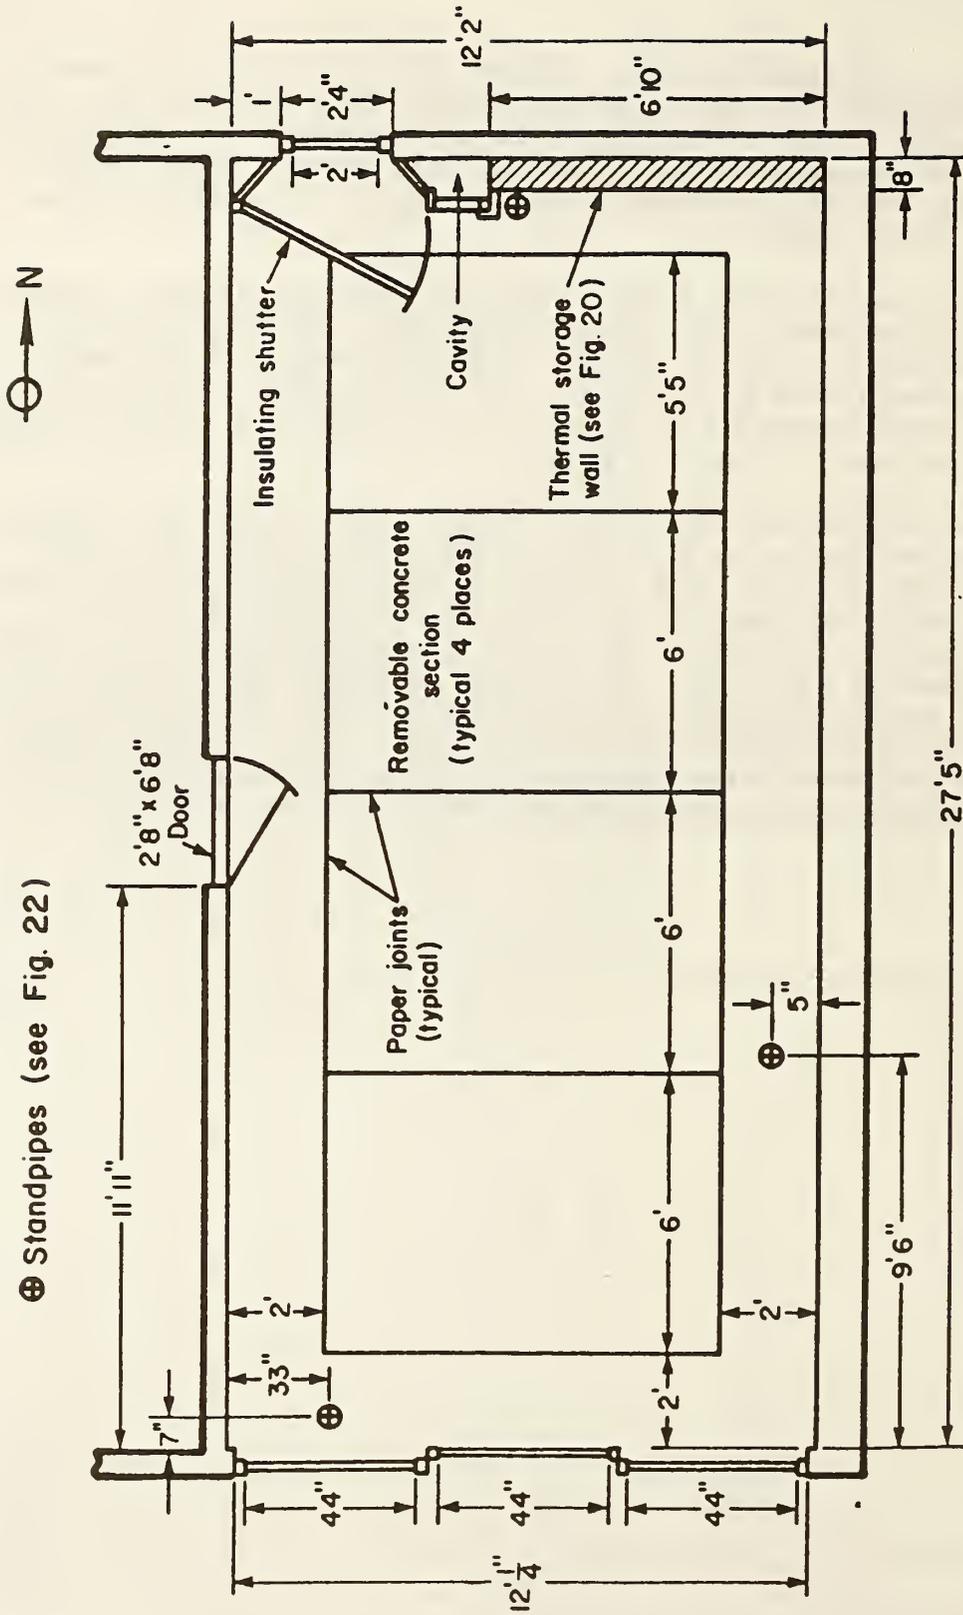


Figure 21. Floor Plan of the Direct Gain Cell (Cell #4)


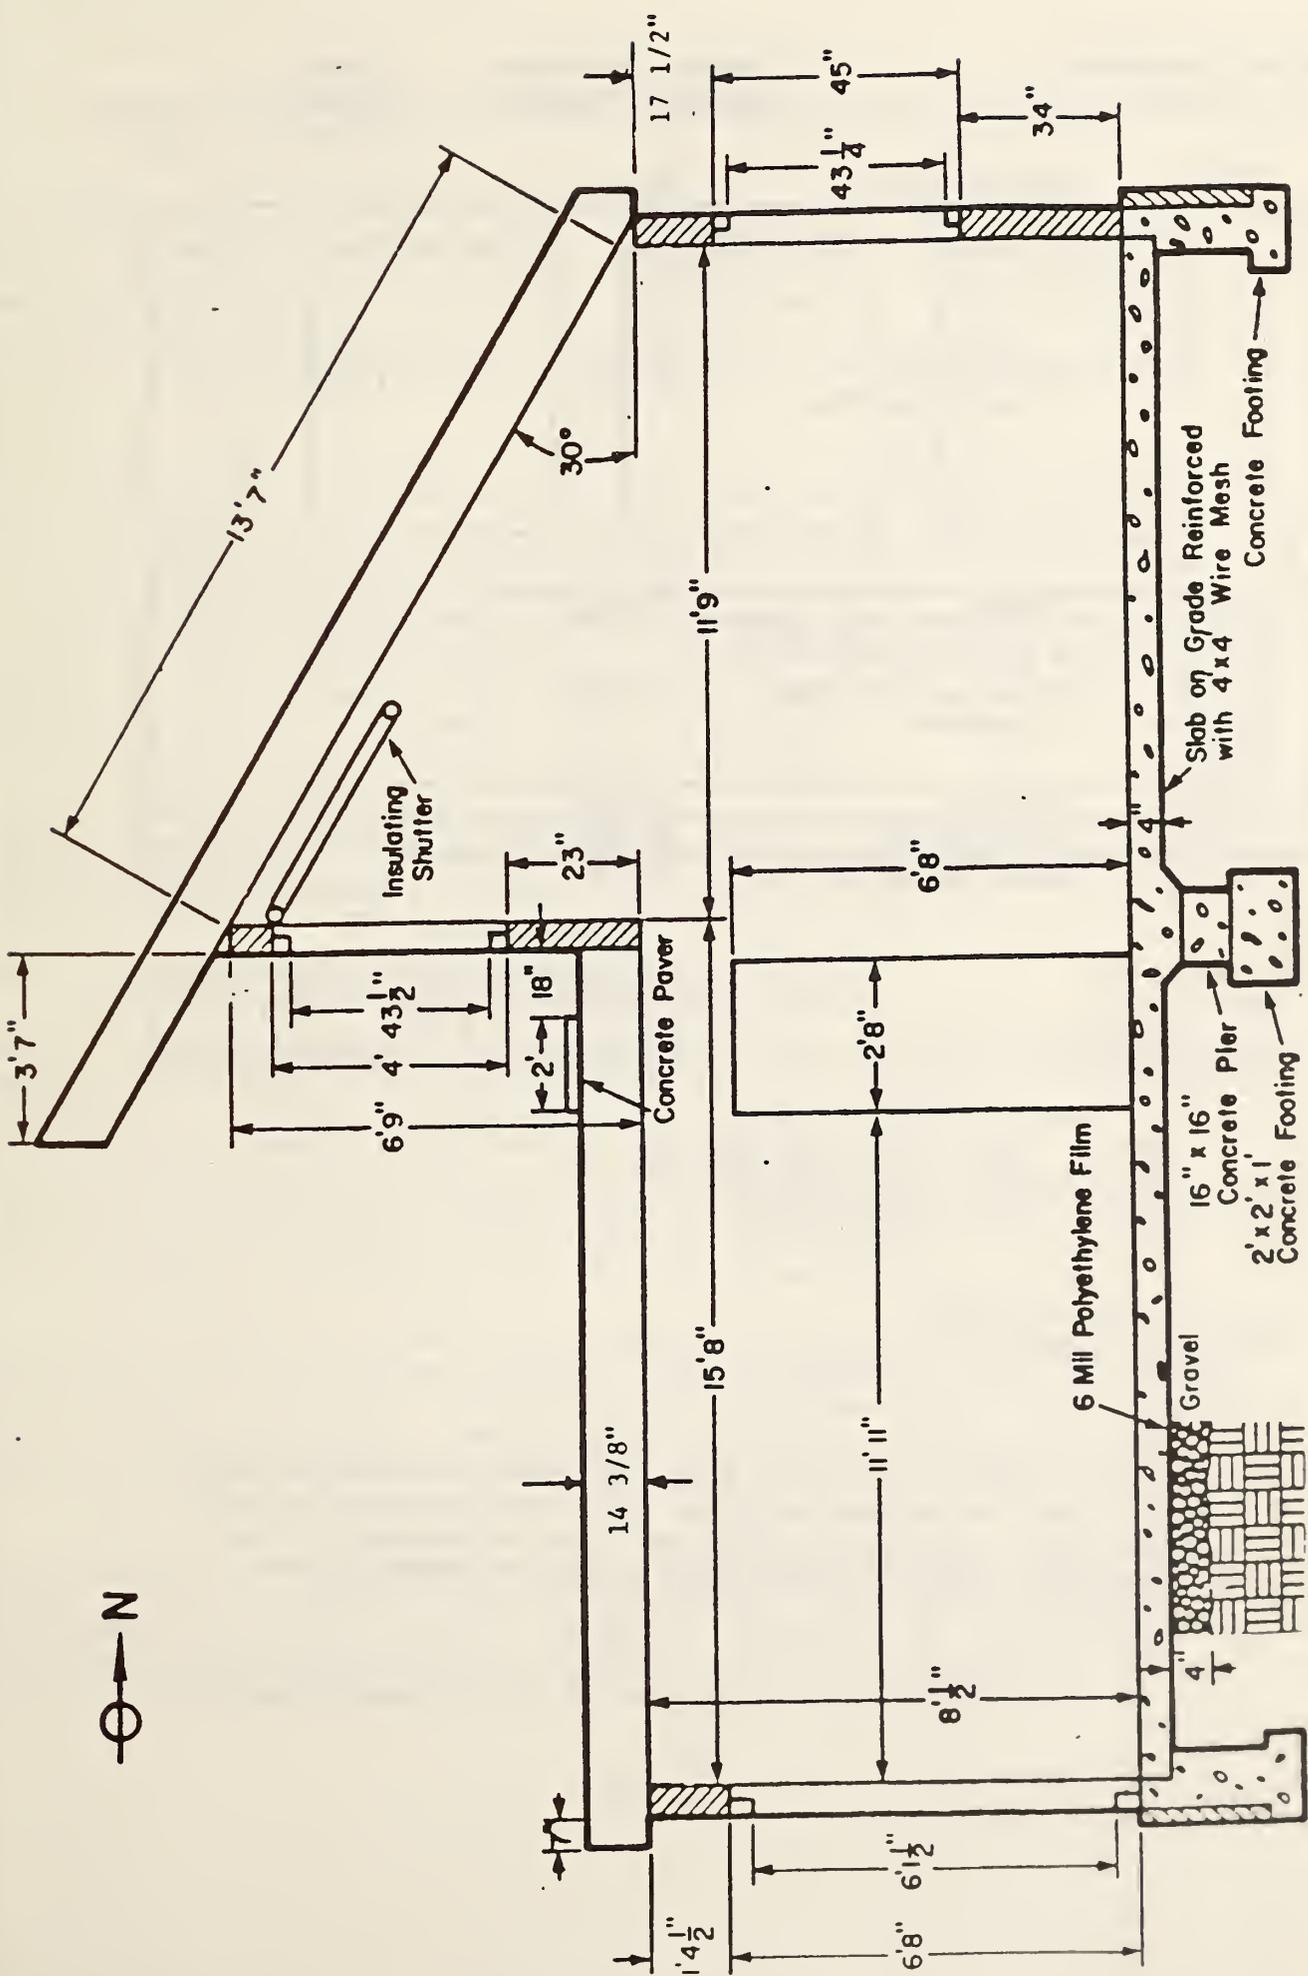


Figure 22. Longitudinal Section of the Direct Gain Cell

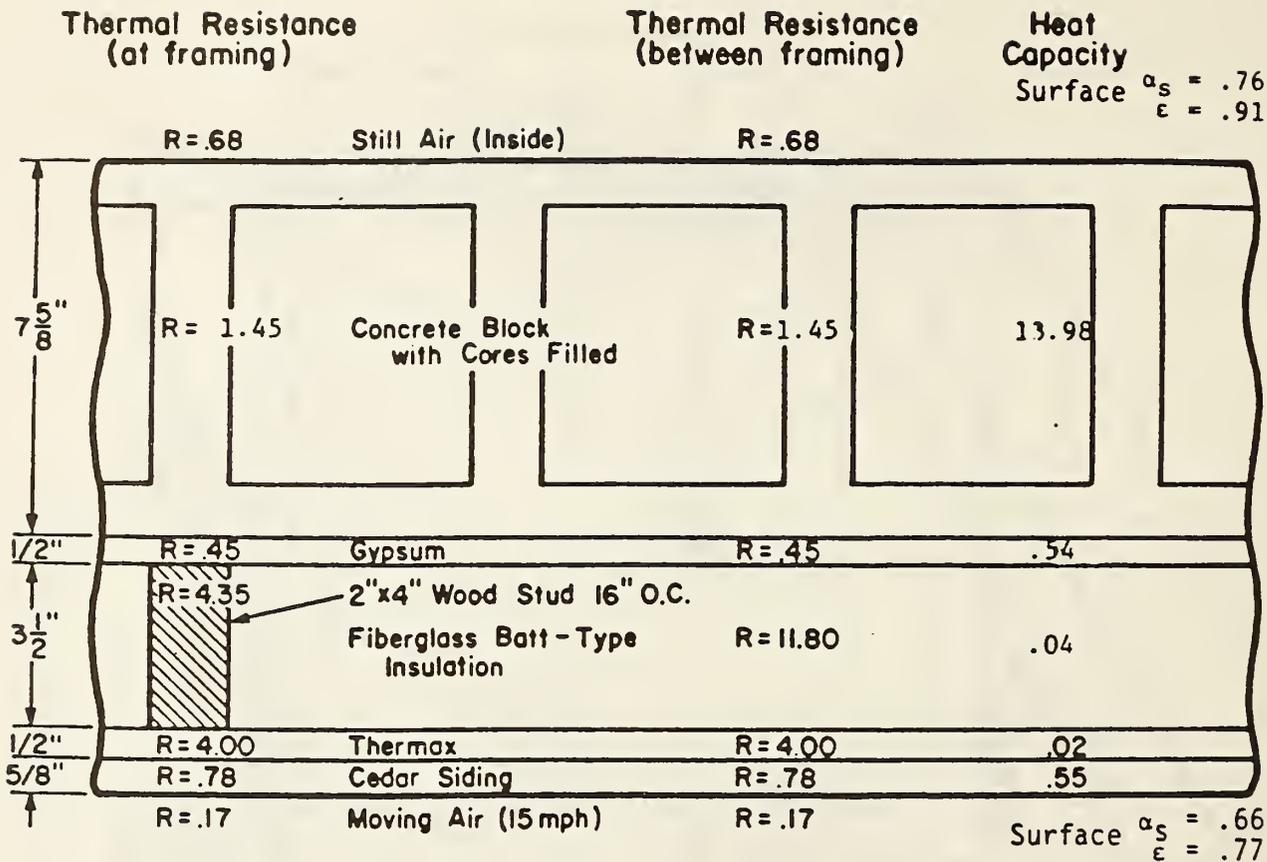

$$R_s = 11.83$$

$$\text{Area} = 15\%$$

$$R_i = 19.33$$

$$\text{Area} = 85\%$$

$$\frac{mCp}{A} = 15.13 \text{ Btu/ft}^2 \text{ } ^\circ\text{F}$$

$$(309.2 \text{ KJ/m}^2 \text{ } ^\circ\text{C})$$

$$U_{AV} = \frac{.15}{11.83} + \frac{.85}{19.33} = .0567 \text{ Btu/ft}^2 \text{ hr } ^\circ\text{F}$$

$$(.3213 \text{ W/m}^2 \text{ } ^\circ\text{C})$$

$$R_{AV} = 17.65 \text{ ft}^2 \text{ hr } ^\circ\text{F/Btu}$$

$$(3.112 \text{ m}^2 \text{ } ^\circ\text{C/W})$$

Note: Although the studs are 16" from center to center, in calculating R values, they are assumed to occupy 15% of the wall area in order to compensate for multidirectional heat flow and because of the additional studs used in corners and as top and bottom plates.

Figure 23: Cross Section of the Thermal Storage Wall

3.7 MATERIALS PROPERTIES AND HEAT LOSS COEFFICIENTS OF THE TEST CELLS

Properties of various building materials are summarized in table 2 and 3. These properties, when not measured, are taken from the ASHRAE Handbook of Fundamentals, 1981. Although the values of thermal resistance and heat capacity are given to two decimal places it should be noted that this degree of accuracy is not necessarily known. In fact, the material properties can vary with ambient temperature and humidity, as well as with the age of the products. Also there is an uncertainty in the fraction of the wall area that is occupied by wood framing (see the note at the bottom of figures 7, 8, and 23.

In determining a total R-value for the wall, a thermal resistance of $.03 \text{ m}^2\text{C/W}$ ($.17 \text{ ft}^2\text{hr}^\circ\text{F/Btu}$) was chosen for "moving air" on the outside wall surfaces. This corresponds to a wind speed of 24 km/h suggested by ASHRAE for winter calculations. (The thermal resistance suggested for summer is $.044$ corresponding to a wind speed of 12 km/h.) Some users of this manual may want to substitute a different value corresponding to the actual measured wind speed. Another "correction" that some users may want to include is the fact that 12.7 mm plywood was used instead of Thermax sheathing within 1.2 m of all exterior corners for structural purposes. (Thus, the R-value of $.704$ should be replaced by an R-value of 11 for the corners of the building.)

The values of overall heat loss coefficient "UA" for various components or heat transfer surfaces of cells #2, #3, and #4 are estimated by using the ASHRAE steady-state method and the material properties discussed above. The values of "UA" are presented in table 4.

3.8 HEATING, VENTILATING, AND AIR-CONDITIONING SYSTEM

Auxiliary heating and cooling is provided with a fan coil unit installed in each cell under the north window. The location of the fan coil unit is shown in figure 10. Heating is provided by a 3.76 kW, 208 V electric heater in the fan coil unit. Cooling is provided by diverting the flow of fluid to the cooling coil of the fan coil unit. The flow of the chiller fluid from the bypass loop is diverted by a solenoid control diverter valve which is actuated by the cooling thermostat. The chiller fluid, a 50-50 water and propylene glycol solution, is chilled by a 2.64 kW air cooled chiller.

The space temperature in each cell is controlled by positive off-setting thermostats with $\pm 0.5^\circ\text{C}$ deadbands. Each cell has two thermostats, one for cooling and the other for heating. The power supply to the heater and diverter valve can be cut off if desired. Also the power supply to the heater and the diverter valve is wired via an interlock system so that the auxiliary heating and cooling cannot be supplied simultaneously.

In addition, two destratifying fans are placed near the center of the floor of cell #4. One fan takes the room air from the floor level and discharges it at the sloped ceiling level near the clerestory window; and the other fan does the reverse. The combined action of the two fans causes the room air to mix and reduce stratification.

Table 2. Material Properties^a
(SI Units)

MATERIALS	α_s	ϵ	k (W/m-°C)	ρ (kg/m ³)	C_p (J/kg-°C)	R (m ² -°C/W)
Gypsum board (127 cm)	0.23 ^c	0.78 ^c	0.161	801	1089	0.079
Gypsum board (1.59 cm)	0.23 ^c	0.78 ^c	0.161	801	1089	0.099
Themax (1.27 cm) ^b - foil- backed polyurethane board	--	--	0.017	28.8	837	0.704
Cedar siding (1.59 cm)	0.66 ^c	0.77 ^c	0.115	513	1382	0.137
Concrete slab (13.72 cm)	0.67 ^c	0.92 ^c	1.42 ^c	2243 ^c	837	0.072 ^c
CMU storage wall (19.37 cm)	0.76 ^c	0.91 ^c	0.76 ^d	1762 ^d	837	0.255 ^d
Fiberglass batt insulation (8.89 cm)	--	--	0.043	9.6	837	2.08
Fiberglass batt insulation (15.24 cm)	--	--	0.025	9.6	837	3.59
Extruded polystyrene (5.05 cm)	--	--	0.029	28.8	1214	1.76
Extruded polystyrene (1.91 cm)	--	--	0.029	28.8	1214	0.660
Soil (Dry)	0.20	0.90	0.35	721	1842	--
Plywood (1.27 cm)	--	--	0.115	545	1214	0.109
Plywood (1.91 cm)	--	--	0.115	545	1214	0.164
Asphalt shingles	0.90	0.90	--	1121	1256	0.077
Roof, gravel or slag (4.45 cm)	0.60	0.90	1.44	888	1675	0.030
Wood (8.81 cm)	--	--	0.155	513	1382	0.329
Interior metal door (4.45 cm)	--	0.90	0.097	881	544	0.44
Louvered door ^d	--	--	0.078	224	1382	0.18
Gravel (10.16 cm layer beneath floor slab)	--	--	1.44	881	1675	0.070

Movable insulation - thermal resistance - 1.23 m²-°C/W

Schedule - In place sundown to sunrise (operated manually)

^a Material properties are taken from ASHRAE Handbook of Fundamentals, 1981, except as otherwise noted. Several of these values will be replaced by measured values as they become available.

^b Material properties estimated.

^c Properties measured.

^d Properties measured for mortar in cores and for remainder of CMU block; Composite CMU block value calculated from these properties.

Table 3. Material Properties^a
(English Units)

MATERIALS	α_s	ϵ	k (Btu/h-ft-°F)	ρ (lb/ft ³)	C_p (Btu/lb-°F)	R (h-ft ² -°F/Btu)
Gypsum board (0.5 in)	0.23 ^c	0.78 ^c	0.093	50.0	.26	0.45
Gypsum board (0.63 in)	0.23 ^c	0.78 ^c	0.093	50.0	.26	0.56
Themax (0.5 in.) ^b - foil- backed polyurethane board	—	—	0.010	1.8	.20	4.00
Cedar siding (0.63 in)	0.66 ^c	0.77 ^c	0.0667	32.0	.33	0.78
Concrete slab (0.45 ft)	0.67 ^c	0.92 ^c	0.82 ^c	140 ^c	.20	0.41 ^c
CMU storage wall (7.63 in)	0.76 ^c	0.91 ^c	0.44 ^d	110 ^d	.20	0.45 ^d
Fiberglass batt insulation (3.5 in)	—	—	0.025	0.6	.20	11.8
Fiberglass batt insulation (6 in)	—	—	0.0250	0.6	.20	20.4
Extruded polystyrene (2 in)	—	—	0.017	1.8	.29	10.0
Extruded polystyrene (0.75 in)	—	—	0.017	28.8	.29	3.75
Soil (dry)	0.20	0.90	~ 0.20	45	.44	—
Plywood (0.5 in)	—	—	0.0667	34	.29	0.62
Plywood (0.75 in)	—	—	0.9667	34	.29	0.93
Asphalt shingles	0.90	0.90	—	70	.30	0.44
Roof, gravel or slag (1.75 in)	0.60	0.90	0.834	55	.40	0.17
Wood (1.5 in)	—	—	0.0667	32	.33	1.87
Interior metal door (1.75 in)	—	0.90	0.056	55	.13	0.44
Louvered door ^b	—	—	0.045	14	.33	1.0
Gravel (10.16 cm layer beneath floor slab)	—	—	0.834	55	.40	0.40

Movable insulation - thermal resistance - 7.0 h-ft²-°F/Btu
Schedule - In place sundown to sunrise (operated manually)

^a Material properties are taken from ASHRAE Handbook of Fundamentals, 1981, except as otherwise noted. Several of these values will be replaced by measured values as they become available.

^b Material properties estimated.

^c Properties measured.

^d Properties measured for mortar in cores and for remainder of CMU block; Composite CMU block value calculated from these properties.

Table 4. Values of Overall Heat Loss Coefficient (UA) Estimated by ASHRAE Steady-State Method.

Item #	Component or Heat Transfer Surface	Overall Heat Loss Coefficient (UA) W/°C (Btu/hr-°F)		
		Cell #2	Cell #3	Cell #4
1.	Ceiling	5.78 (3.05)	5.78 (3.05)	5.78 (3.05)
2.	Floor	4.70 (2.48)	4.70 (2.48)	10.10 (5.33)
3.	East wall	0.00 *	0.00 *	4.92 (2.60)
4.	West wall	0.00 *	0.00 *	0.00 *
5.	North wall	3.49 (1.84)	3.49 (1.84)	3.49 (1.48)
6.	Upper level south wall with clerestory shutter:			
	a. closed	4.23 (2.23)	4.23 (2.23)	4.23 (2.23)
	b. open	18.0 (9.50)	18.0 (9.50)	18.0 (9.50)
7.	Lower level south wall.	14.45 (7.63)	9.58 (5.06)	28.15 (14.8)

* The UA value of the inside partition walls is equal to 7.95 W/°C (4.20 Btu/hr-°F). However, for the purpose of estimated UA value for the test cells the inside partition walls are considered to have a UA value of zero. This is so because the cell temperatures for the duration of an experiment, are nearly equal and the intercell heat transfer is negligible in comparison to heat transfer through the other surfaces.

4. INSTRUMENTATION

A total of 457 sensors are installed in and around the building. There are 26 sensors outside the building, and 6, 173, 26, and 226, respectively, are in cell #1, cell #2, cell #3, and cell #4. These include flow meters, heat flux meters, pyrometers, resistance thermometers, thermocouples, watt-hour meters, and weather sensors. The general location of these sensors is summarized in table 5.

The sensors in this handbook are labeled by a letter and a number. The letters include H (radiation), Q (heat flux), R (resistance thermometer), T (temperature), W (weather), and WH (watt-hour). The number, for the sensors installed prior to FY83, correspond to the sensor in references 1 and 5. The sensors labeled T267 to T271 in cell #2 in reference 1 have been removed and replaced by new sensors. The sensors labeled T400 to T520 were installed in FY83 and FY84. The details of the sensor locations are described below.

4.1 OUTSIDE THE BUILDING

There are 4 solar radiation sensors, a ground reflectance sensor, a wind speed and wind direction sensor, and 19 thermocouples outside the building.

A pyrometer (H215) mounted on the lower wall of cell #3, 0.5 m (20 in) from the west of cell #4 and 1.2 m (48 in) above ground is used to measure total radiation on a south vertical surface. Two pyrometers mounted on the upper roof are used to measure sky irradiation (H216) and total horizontal radiation (H217). Ground reflectance is measured by an inverted pyrometer (H218) located about 4 m from the south wall and 5 m (197 in) from the east wall of the building. Normal beam radiation is measured by a pyrliometer (H219) mounted on the lower roof.

The wind speed and wind direction is measured by an anemometer and vane system located about 61 m (200 ft) southwest of the test building.

Four mechanically aspirated and shielded thermocouples are used to measure the outside ambient air temperature. Two of these thermocouples, about 20 mm (.8 in) apart from each other, are about 1.2 m (48 in) above ground and about 2.5 m (99 in) south of the test building; the other two thermocouples are similarly situated on the north of the building. The location of these thermocouples is indicated in figure 1. A ground probe containing 12 thermocouples is used to monitor the ground temperature. The ground probe is located at a distance of 6.7 m (22 ft) from the northwest corner of the building. The location of the outside ground probe is indicated in figure 1, while the details are given in figure 24. The location of the thermocouples for monitoring the outside surface temperatures of east and north walls of cell #4 are shown in figure 25.


Table 5. Various Sensors Installed at the NBS Passive Solar Test Facility

Item #	Sensor Type	General Location and Quantity					
		Outside	Cell #1	Cell #2	Cell #3	Cell #4	
1	Flow meters (chiller fluid)*			1	1	1	
2	Heat flux meters						11
3	Resistance thermometers			2	2	2	
4	Radiation sensors						
4.1	Direct normal beam	1					
4.2	Ground reflectance	1					
4.3	Infrared sky radiation	1					
4.4	Total horizontal	1					
4.5	Total on a south vertical surface	1					1
5	Type-T thermocouples						
5.1	Air	4		23	3	25	55
5.2	Black globe			3		5	8
5.3	Ceiling surface			12		12	24
5.4	East wall surface	2		3		13	18
5.5	Floor surface			12	20	12	44
5.6	Foundation			18*		54	72
5.7	Ground	12		11		46	69
5.8	Heat flux meter surface					11	11
5.9	Heater discharge					1	1
5.10	North wall	1		3		16	20
5.11	Pink globe					2	2
5.12	Trombe wall			82			82
5.13	West wall			3		13	16
6	Watt-hour meters		6				6
7	Weather sensor						
7.1	Wind direction	1					1
7.2	Wind speed	1					1
	Total	26	6	173	26	226	457

* Currently not monitored.


Ground Probe Sensor Numbers

Inside Probe			Outside Probe		
Sensor	x	Channel	Sensor	x	Channel
A	143 $\frac{1}{4}$	T277	M	143 $\frac{1}{2}$	T500
B	132 $\frac{3}{8}$	T278	N	132 $\frac{1}{8}$	T501
C	120 $\frac{1}{4}$	T279	O	120 $\frac{1}{8}$	T502
D	108 $\frac{3}{8}$	T280	P	108 $\frac{1}{8}$	T503
E	96 $\frac{1}{4}$	T281	Q	96 $\frac{1}{8}$	T504
F	84 $\frac{1}{4}$	T282	R	84 $\frac{1}{16}$	T505
G	72 $\frac{1}{4}$	Broken	S	72 $\frac{1}{8}$	T506
H	60 $\frac{1}{4}$	T283	T	60 $\frac{1}{8}$	T507
I	48 $\frac{1}{8}$	T284	U	48 $\frac{1}{4}$	T508
J	36 $\frac{1}{4}$	T285	V	36 $\frac{1}{8}$	T509
K	24 $\frac{1}{4}$	T286	W	24 $\frac{1}{4}$	T510
L	12 $\frac{1}{4}$	T287	X	12 $\frac{1}{4}$	T511

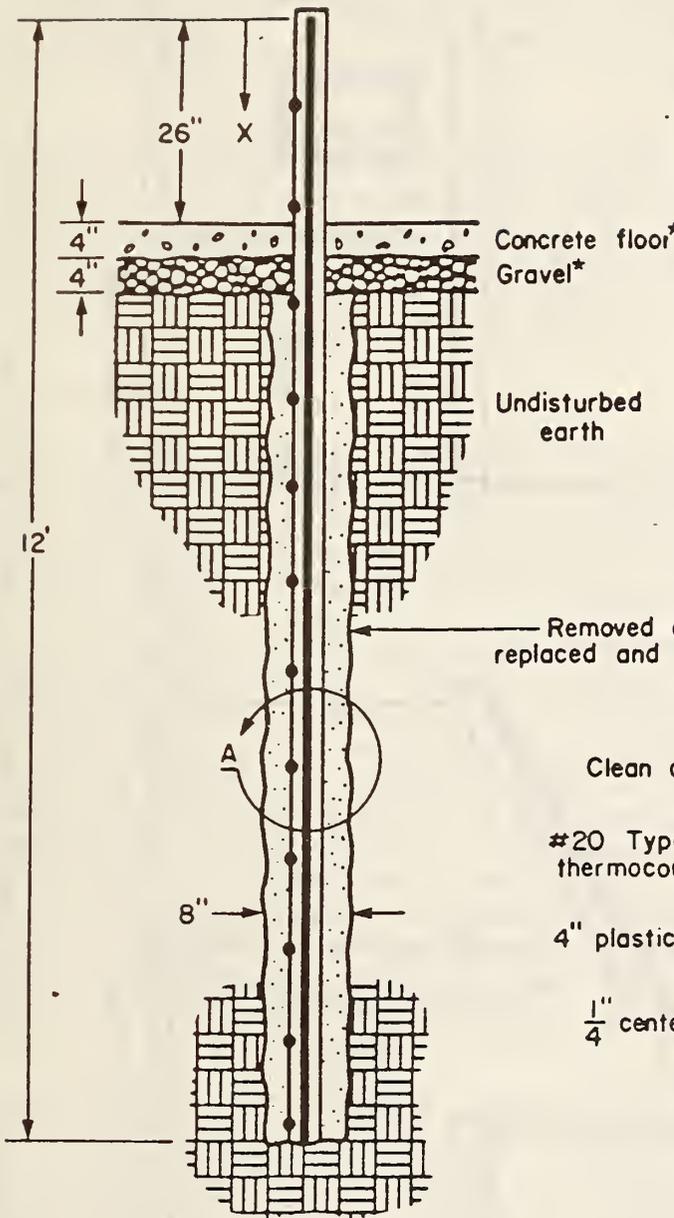


Removed earth replaced and tamped

- Clean dry sand
- #20 Type T thermocouple
- 4" plastic pipe
- $\frac{1}{4}$ " centering dowel

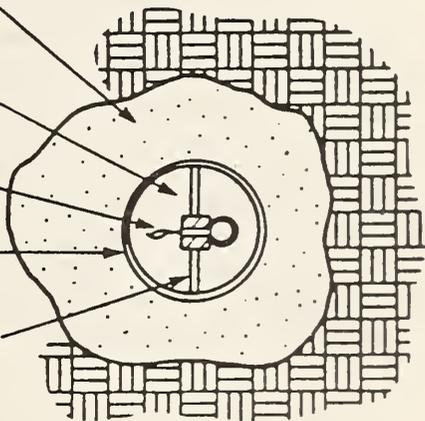


A.

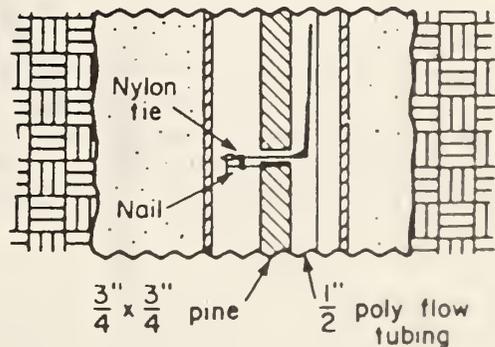

*inside probe only

Figure 24. Ground Temperature Probes
(See Figs. 1 and 16 for locations)

North Elevation

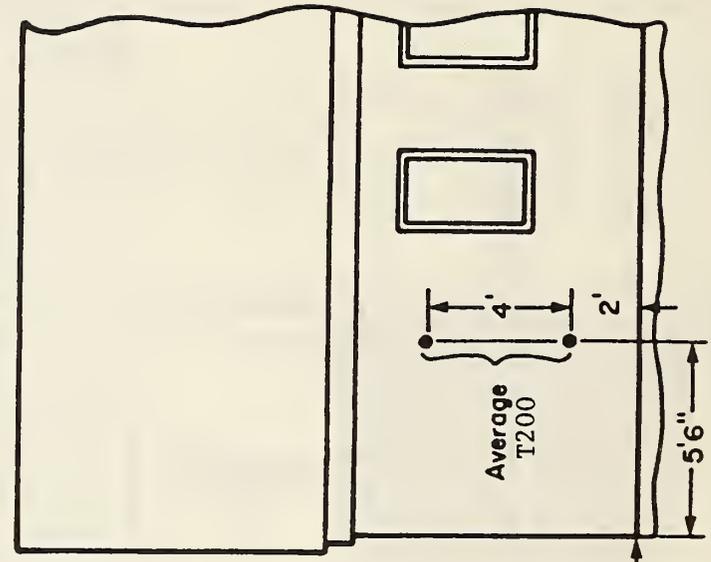

East Elevation

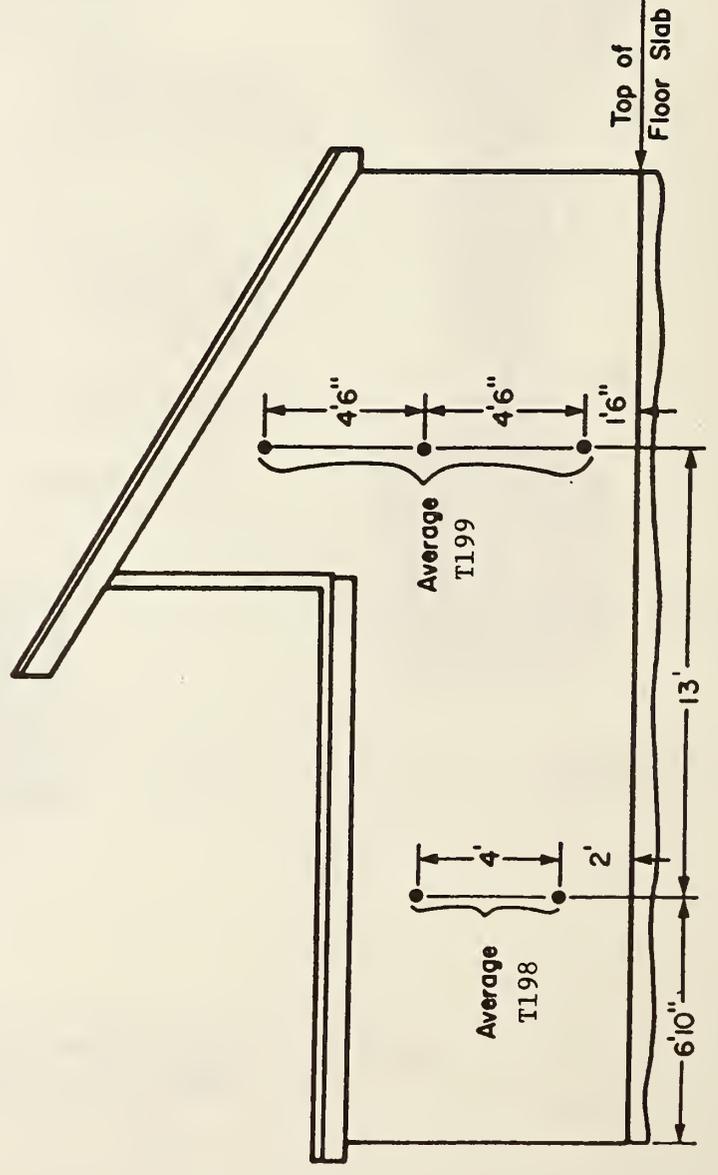


Figure 25. Outside Surface Temperature Sensor Locations (Cell #4)

4.2 CELL #1

As indicated earlier, this cell houses the data acquisition system (DAS), and the continuous air infiltration monitoring system. All of the sensors are connected to the DAS in this cell.

This cell contains 6 watt-hour meters, labeled WH1 to WH6, for monitoring the electrical energy supplied to cells #2, #3, and #4. There are two watt-hour meters for each of the three cells, one for the fan coil unit and one for the lights and electrical outlets. WH1, WH3, and WH5, respectively, are for the fan coil units in cell #2, cell #3, and cell #4; and WH2, WH4, WH6, respectively, are for the lights and outlets in cell #2, cell #3, and cell #4. Also a reference millivolt source is located in the cell #1.

4.3 CELL #2

There are 170 Type T thermocouples, 2 resistance thermometers (RTD), and 1 flow meter placed in this cell. The flow meter, which is not currently monitored, is for measuring the chiller fluid flow rate flowing through the chiller of the fan coil unit. Two RTD's monitor the temperature of the chiller fluid entering (R231) and leaving (R232) the fan coil unit.

The location of the various thermocouples (TC) are shown schematically in figures 18, and 26 to 31. Figure 18 shows the location of 3 TC's on the inner surface of glazing, 3 TC's on the outer surface to Trombe wall, and 4 TC's in the vents (one in each vent) of the Trombe wall. Figure 26 shows the location of 63 TC's embedded in the Trombe wall and 9 TC's on the inside surface of the Trombe wall. Figure 27 shows the location of 22 shielded TC's for cell air temperatures, 3 TC's placed at the center of black globes, (one unshielded TC placed near the thermostats is not shown). A schematic of the radiation shield used for the thermocouples measuring air temperature in cells #2 and #4 is shown in figure 40. Figure 28 shows the location of 12 TC's on the floor surface and 12 TC's on the ceiling surface. Figures 29, 30, and 31, respectively, show the location of 3 TC's on the east wall, 3 TC's on the west wall, and 3 TC's on the north wall of cell #2.

In addition there is a ground probe in cell #2 which is similar to the ground probe situated outside of the test building. The location of the ground probe in cell #2 is indicated in figure 15, while the location of the 11 TC's within the probe has been shown in figure 22. Also the cell contains a foundation probe containing 18 TC's, these thermocouples are not currently monitored. The location of the foundation probe has been indicated in figure 16, the details of the foundation probe and foundation sensor location is given in figure 37 along with the foundation sensors for cell #4.

STORAGE WALL SENSOR NUMBERS

Probe #	Depth From Inside Surface (inch) cm							Inside Surface
	19.05 (7.50)	17.46 (6.88)	13.65 (5.38)	9.84 (3.88)	6.03 (2.38)	2.22 (0.88)	0.32 (0.13)	
1	T288	T289	T290	T291	T292	T293	T294	T465
2	T295	T296	T297	T298	T299	T300	T301	T466
3	T302	T303	T304	T305	T306	T307	T308	T467
4	T309	T310	T311	T312	T313	T314	T315	T462
5	T316	T317	T318	T319	T320	T321	T322	T463
6	T323	T324	T325	T326	T327	T328	T329	T464
7	T330	T331	T332	T333	T334	T335	T336	T459
8	T337	T338	T339	T340	T341	T342	T343	T460
9	T344	T345	T346	T347	T348	T349	T350	T461

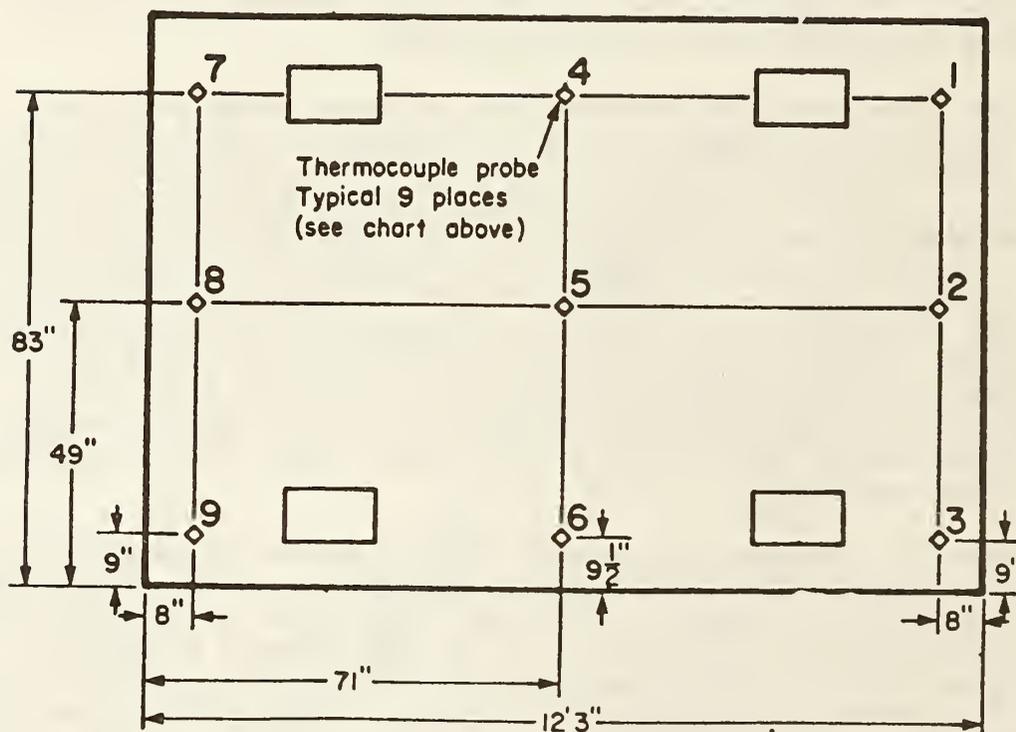


Figure 26. Trombe Wall Sensor Locations in Cell #2

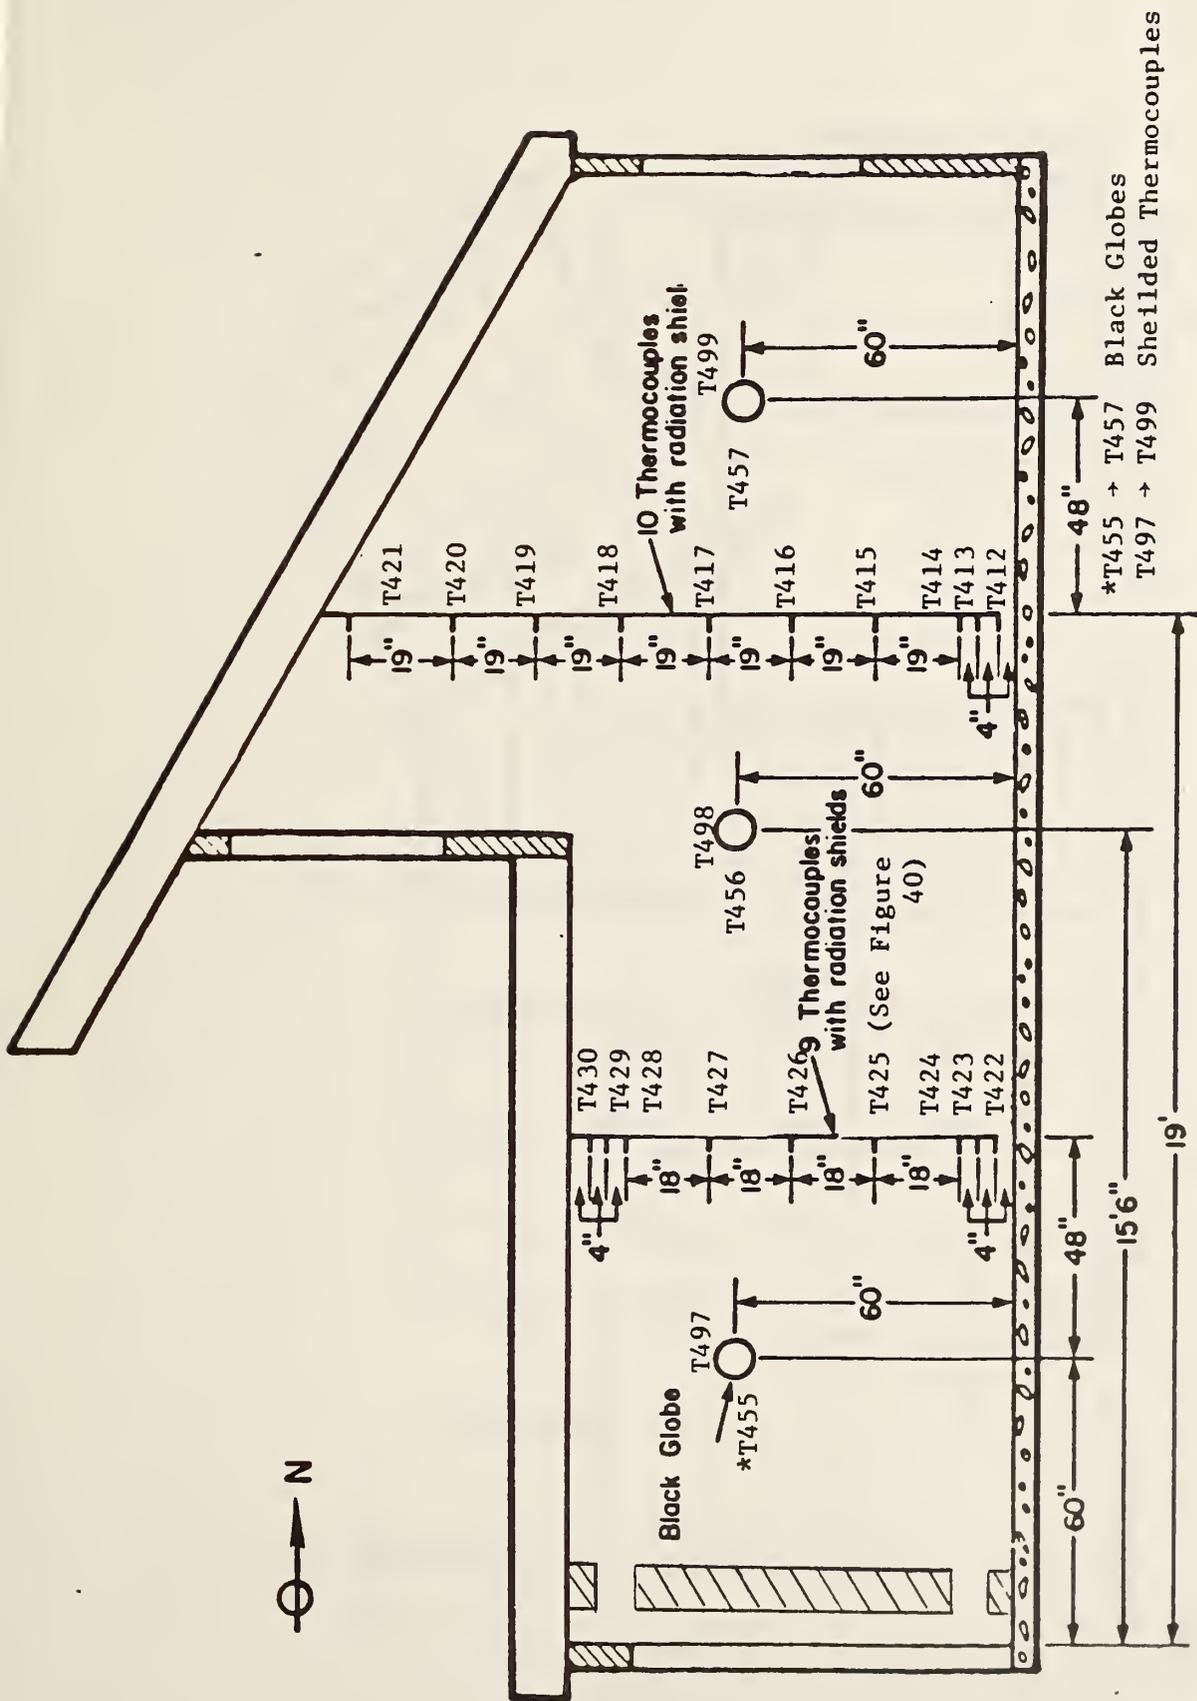


Figure 27. Air Temperature Sensor Locations in Cell #2

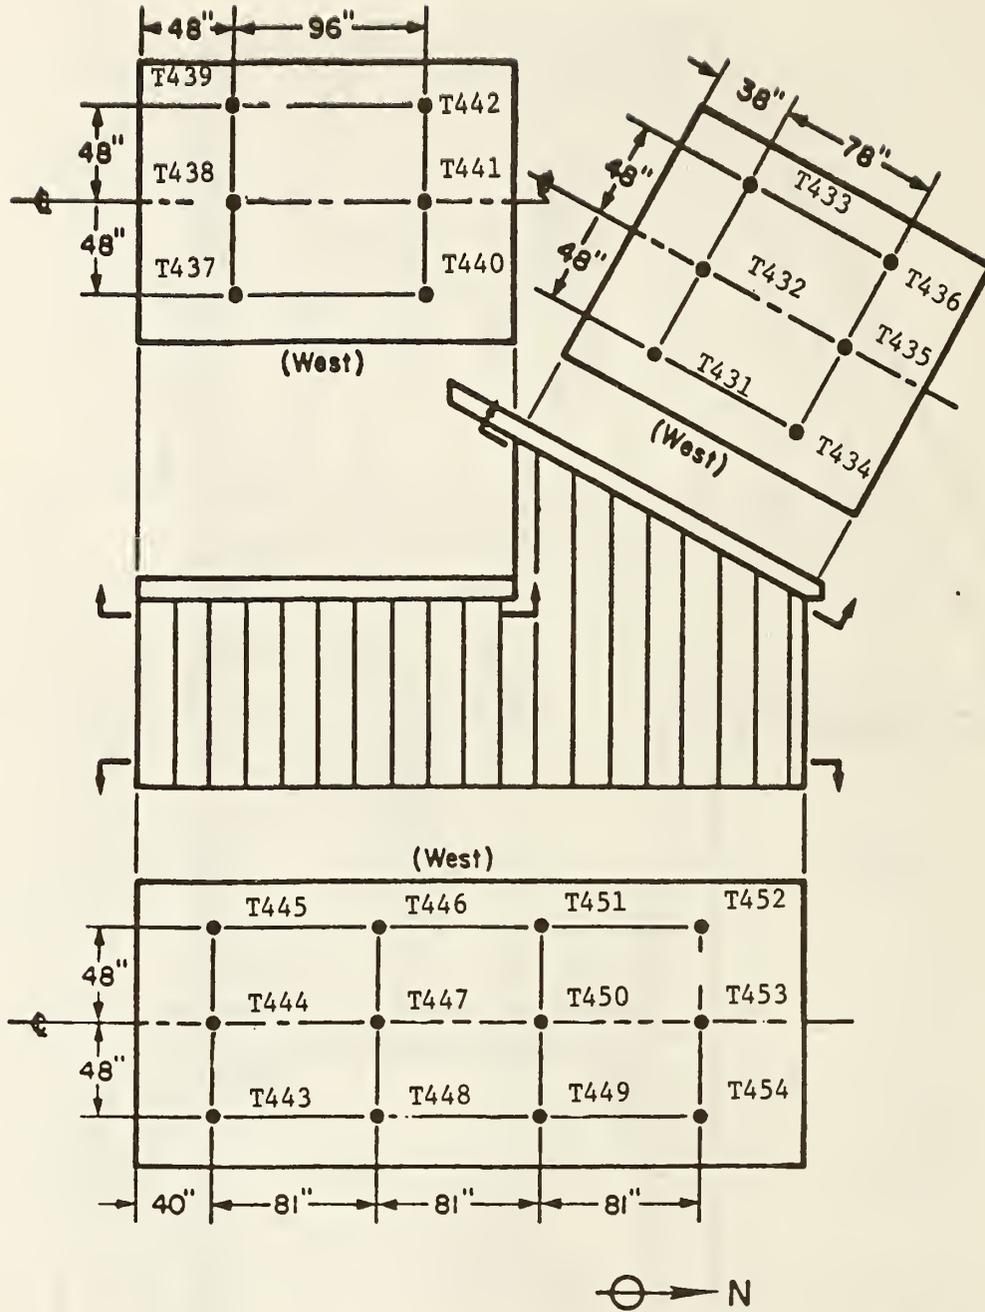


Figure 28. Sensor Locations Floor and Ceiling Cell #2

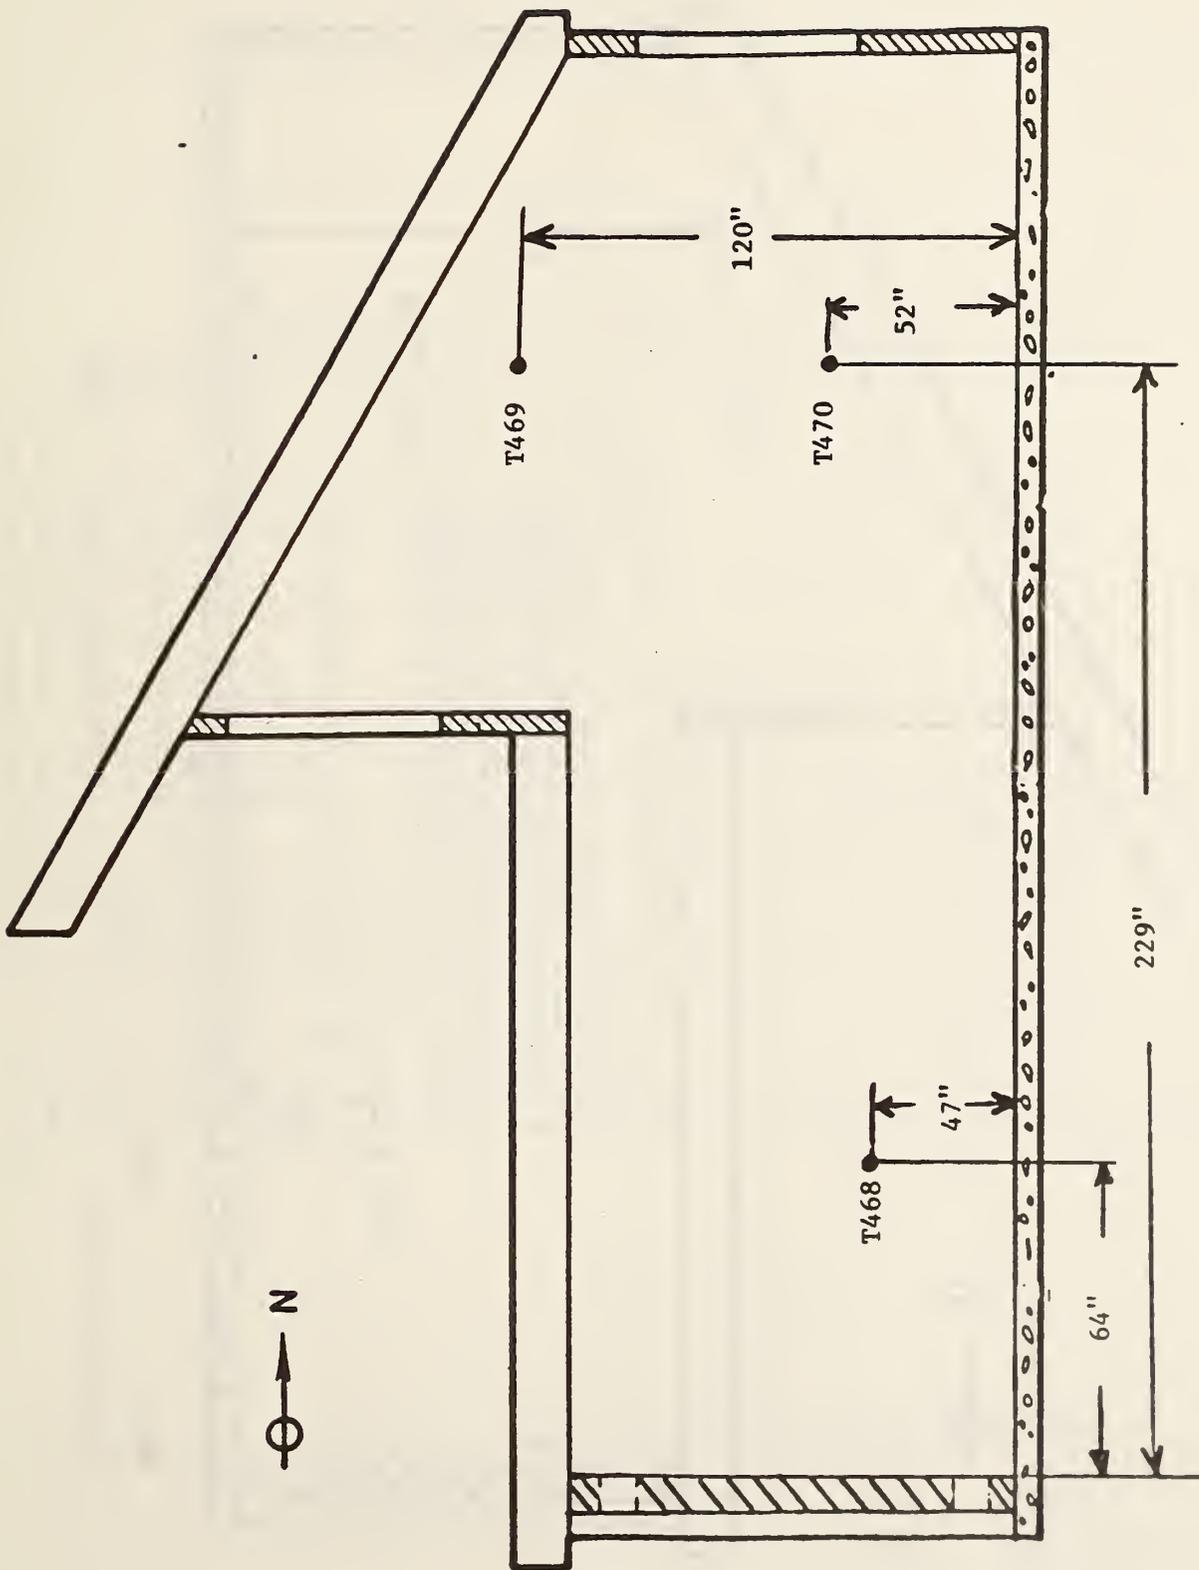


Figure 29. Sensor Locations East Wall Cell #2.

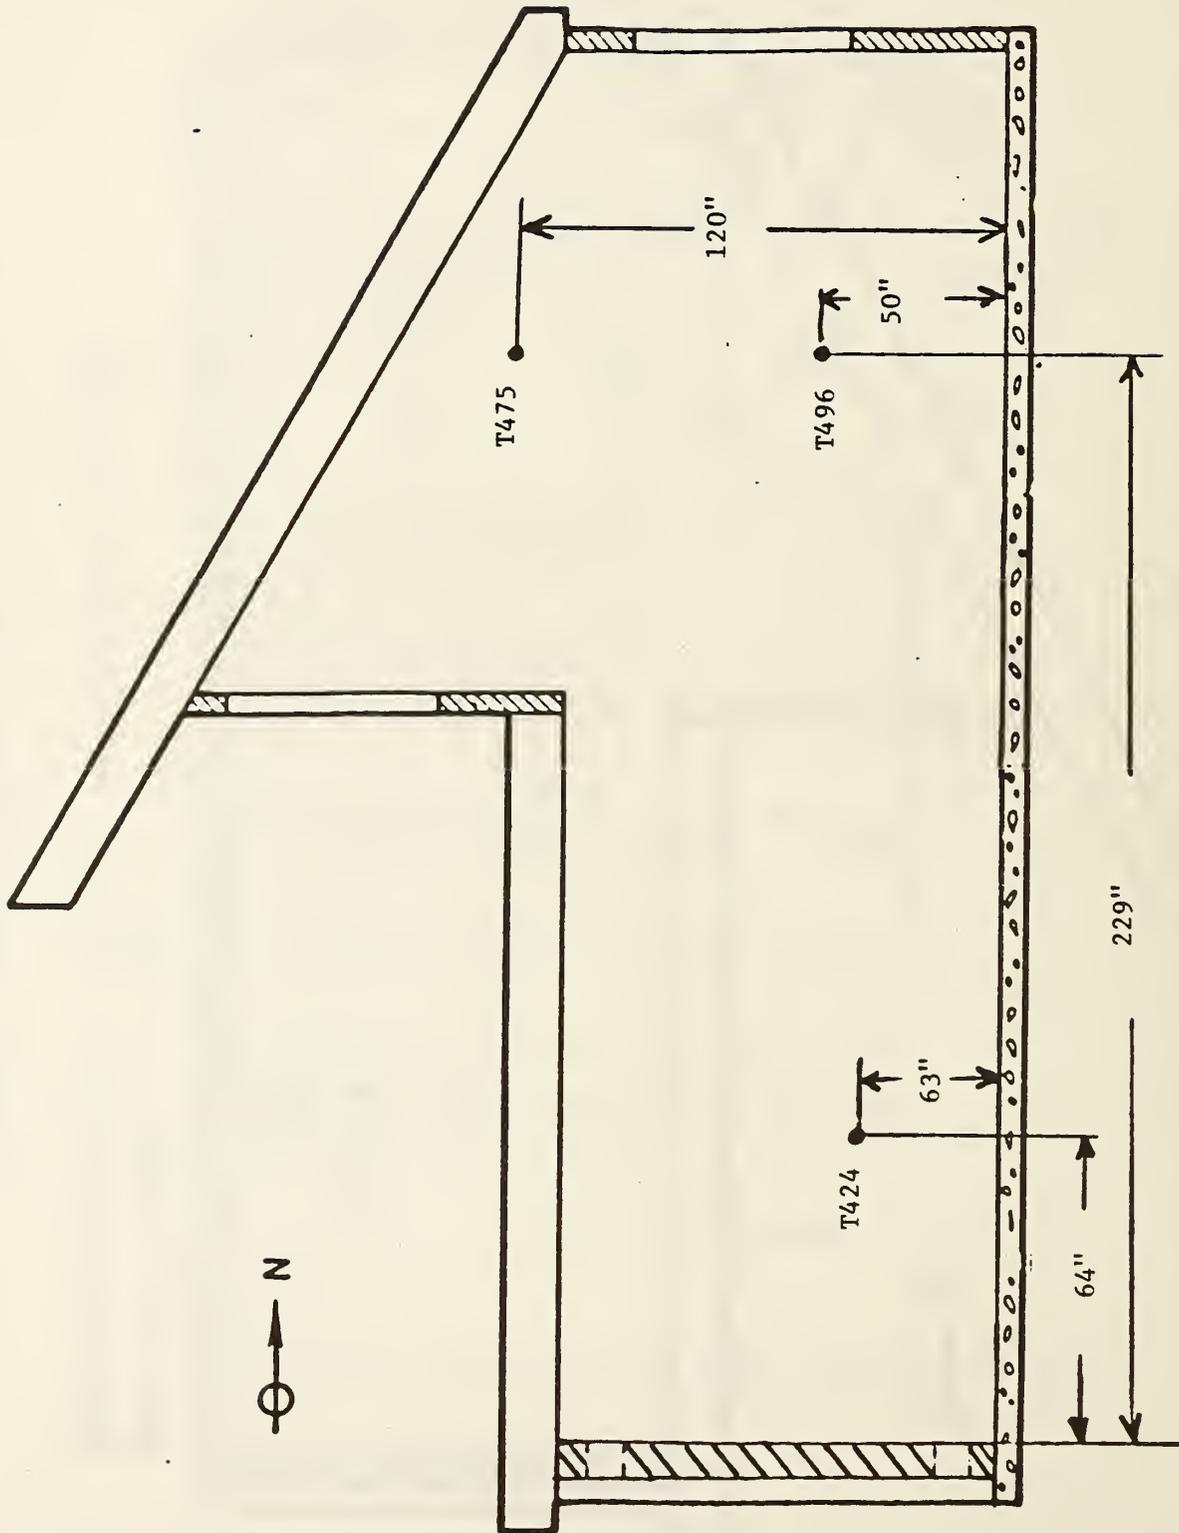


Figure 30. Sensor Locations West Wall Cell #2

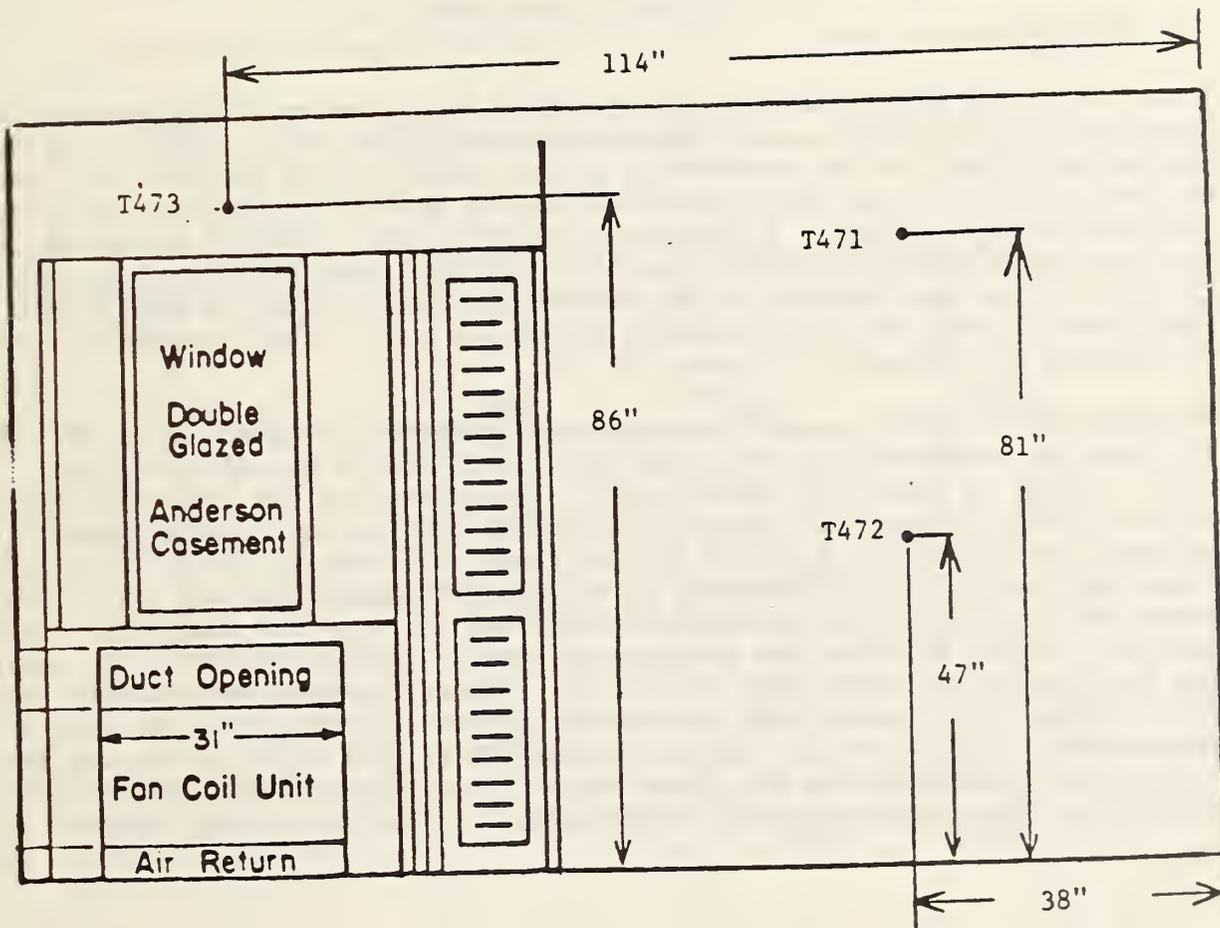


Figure 31. Sensor Locations North Wall Cell #2

4.4 CELL #3

There are 20 TC's to monitor the floor surface temperature in cell #3. Figure 32 schematically shows the location of these sensors. The air temperature in cell #3 is monitored at two locations with unshielded thermocouples, and averaged, see figure 19 for details.

The cell has 2 RTD for monitoring the temperature of the chiller fluid entering (R233) and leaving (R234) the fan coil unit. There also is a flow meter in the cell which is not currently monitored.

4.5 CELL #4

There is a total of 226 sensors in this cell, 1 flow meter, 1 pyronometer, 11 heat flux meters, 3 RTD's, and 210 thermocouples. Two RTD's, R235 and R236, respectively, monitor the temperature of the chiller fluid entering and leaving the fan coil unit. The RTD labeled R237 is for monitoring the room air temperature near the thermostats. A flow meter, which is not currently monitored, is for monitoring the flow rate of the chiller fluid. The pyronometer is placed in front of the west section of the direct gain fenestration to monitor the total south-facing vertical radiation inside the cell. The location of this pyronometer is indicated in figure 39.

The location of other sensors is schematically shown in figures 33 to 39. Figure 33 shows the location of 6 heat flux meters and 19 TC's placed on the east wall. Figure 34 shows the location of 13 TC's placed on the inside surface of the west wall of cell #4. Figure 35 shows the location of various sensors placed on the ceiling (1Q and 13 TC) and floor (2Q's and 14 TC's). Figure 36 shows the details of the placement of 46 ground thermocouples, and figure 37 shows the location of the foundation probes and the location foundation thermocouples. Figure 38 shows the position of various sensors (2 heat flux meters and 18 TC's) on the north wall in cell #4. Figure 39 shows the position of 25 (22 shielded and 3 unshielded) thermocouples used for monitoring the cell air temperature. Figure 39 also shows the location of five black globes and two pink globes used for monitoring the globe temperature. Thermocouple T265, used for monitoring the heater discharge temperature, is not shown in any figure.

All dimensions in inches

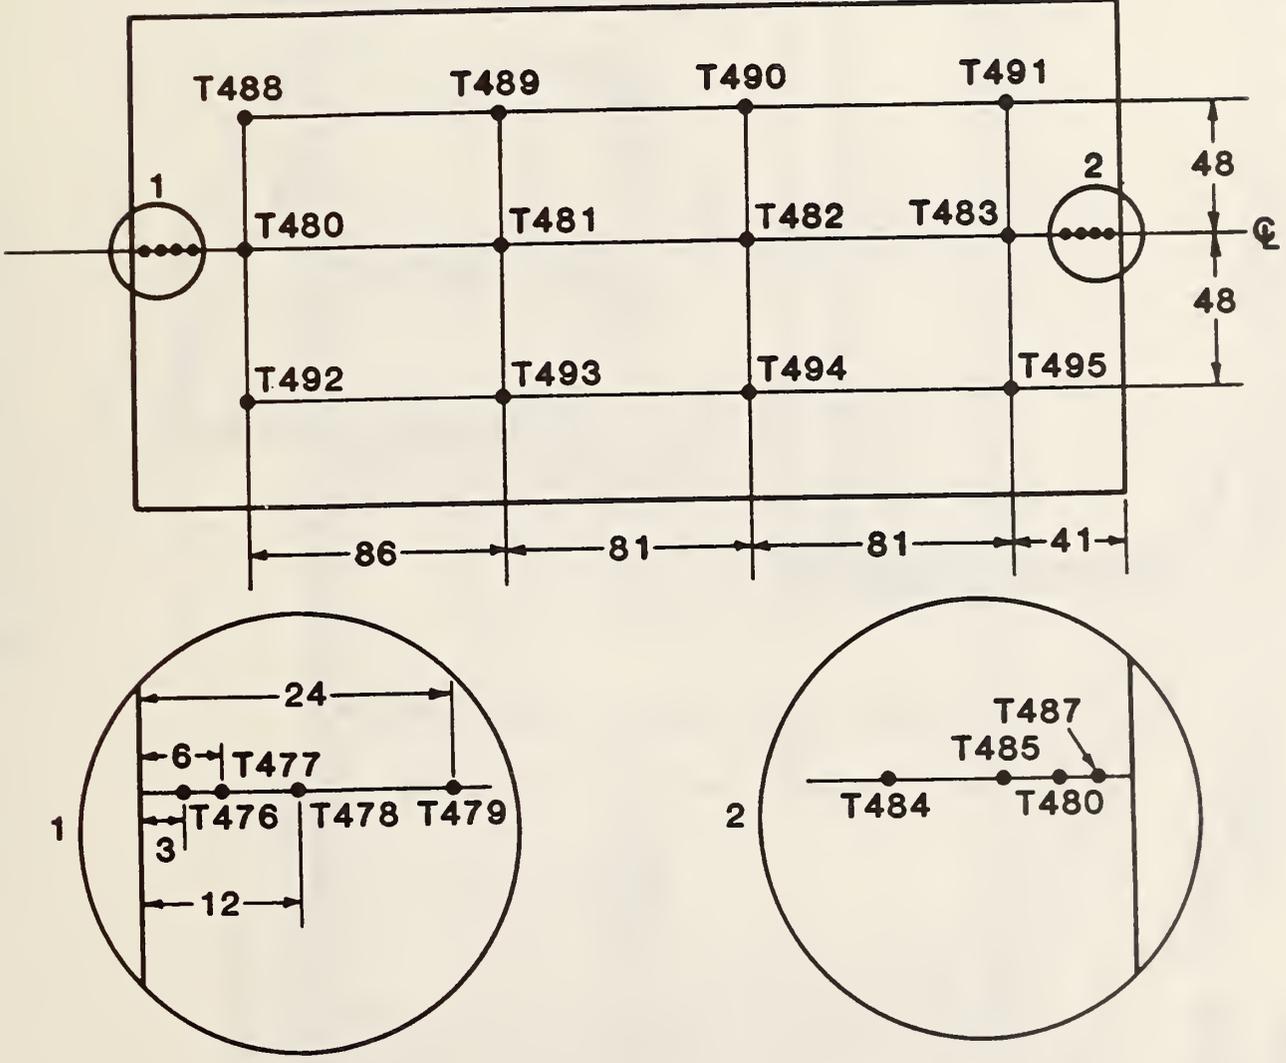


Figure 32. Sensor Locations Floor Surface Cell #3

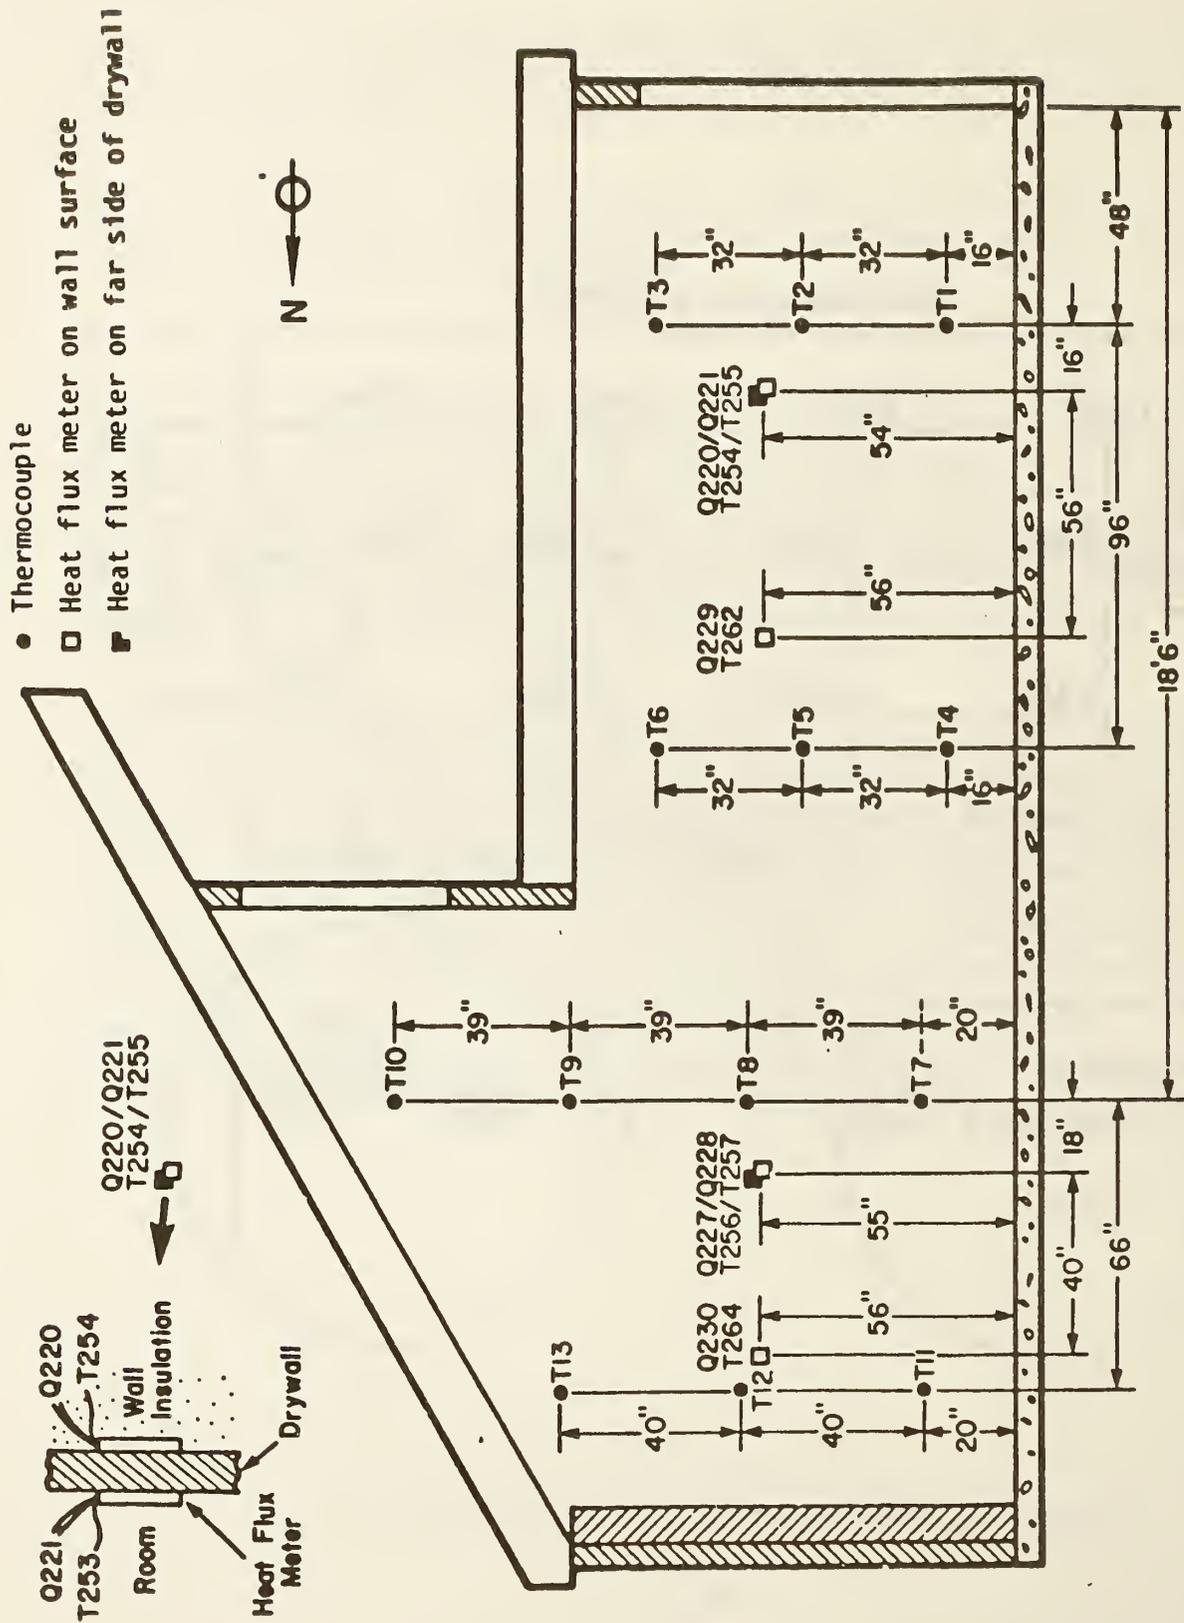


Figure 33. Sensor Locations East Wall Cell #4

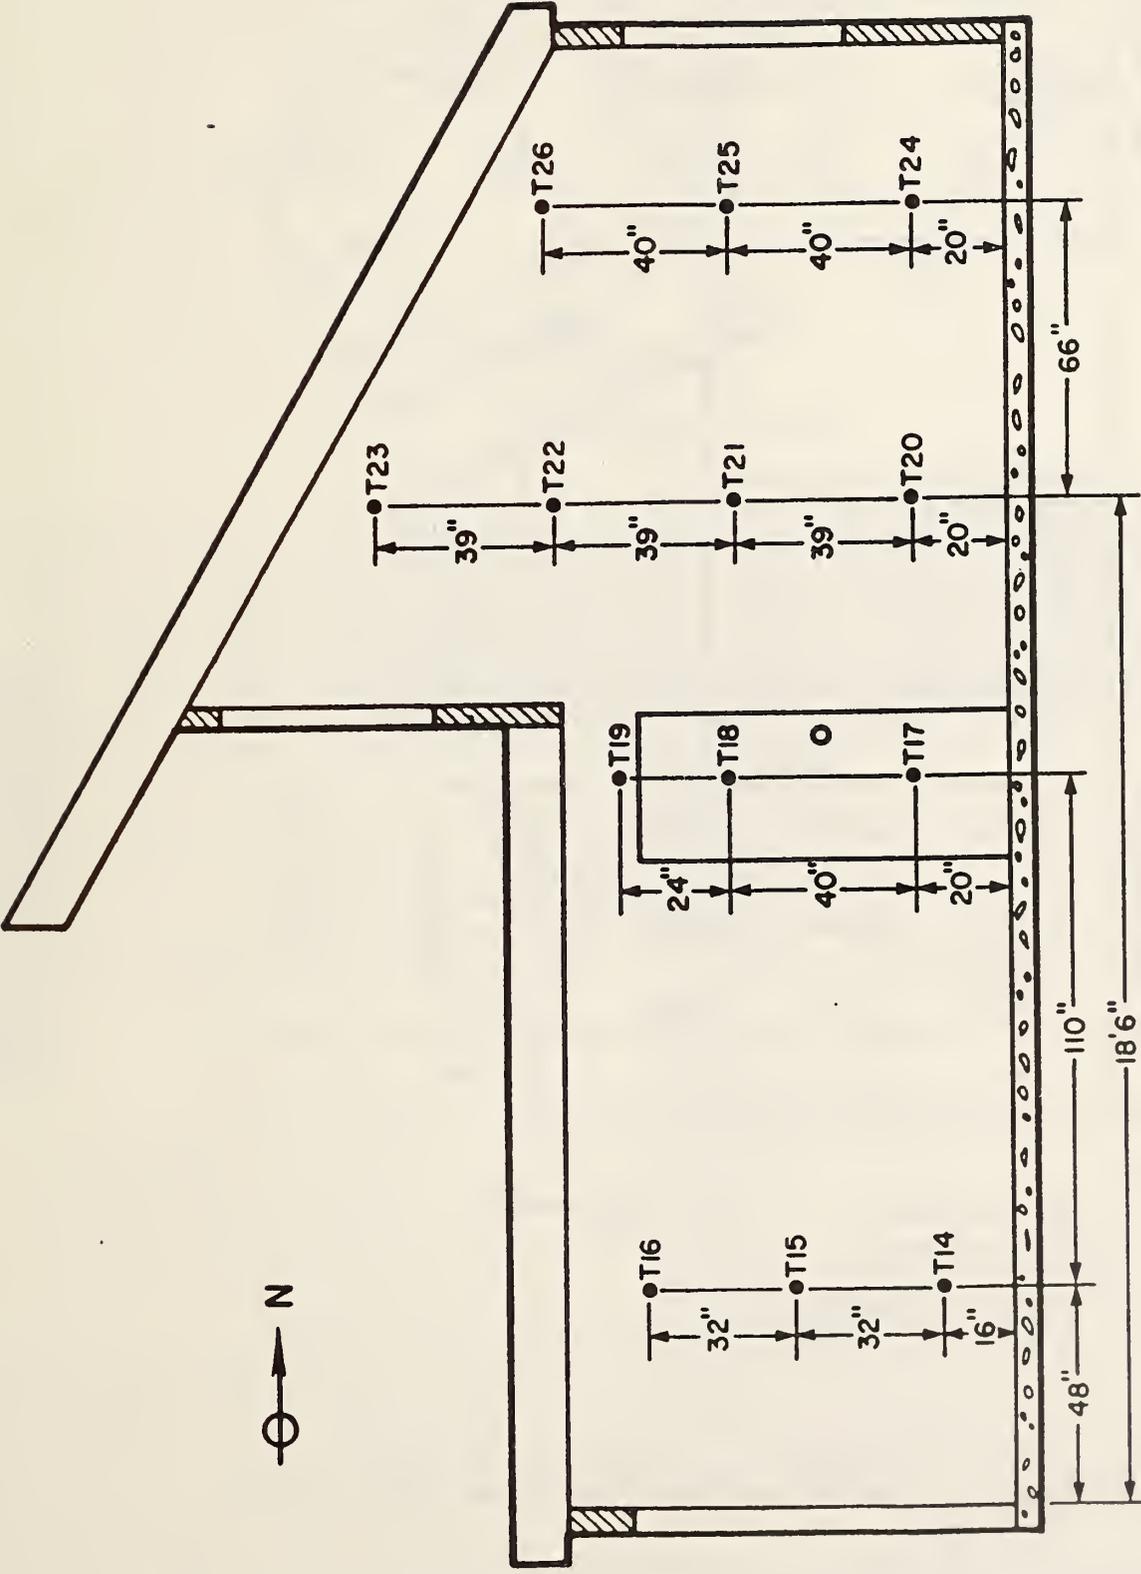


Figure 34. Sensor Locations West Wall Cell #4

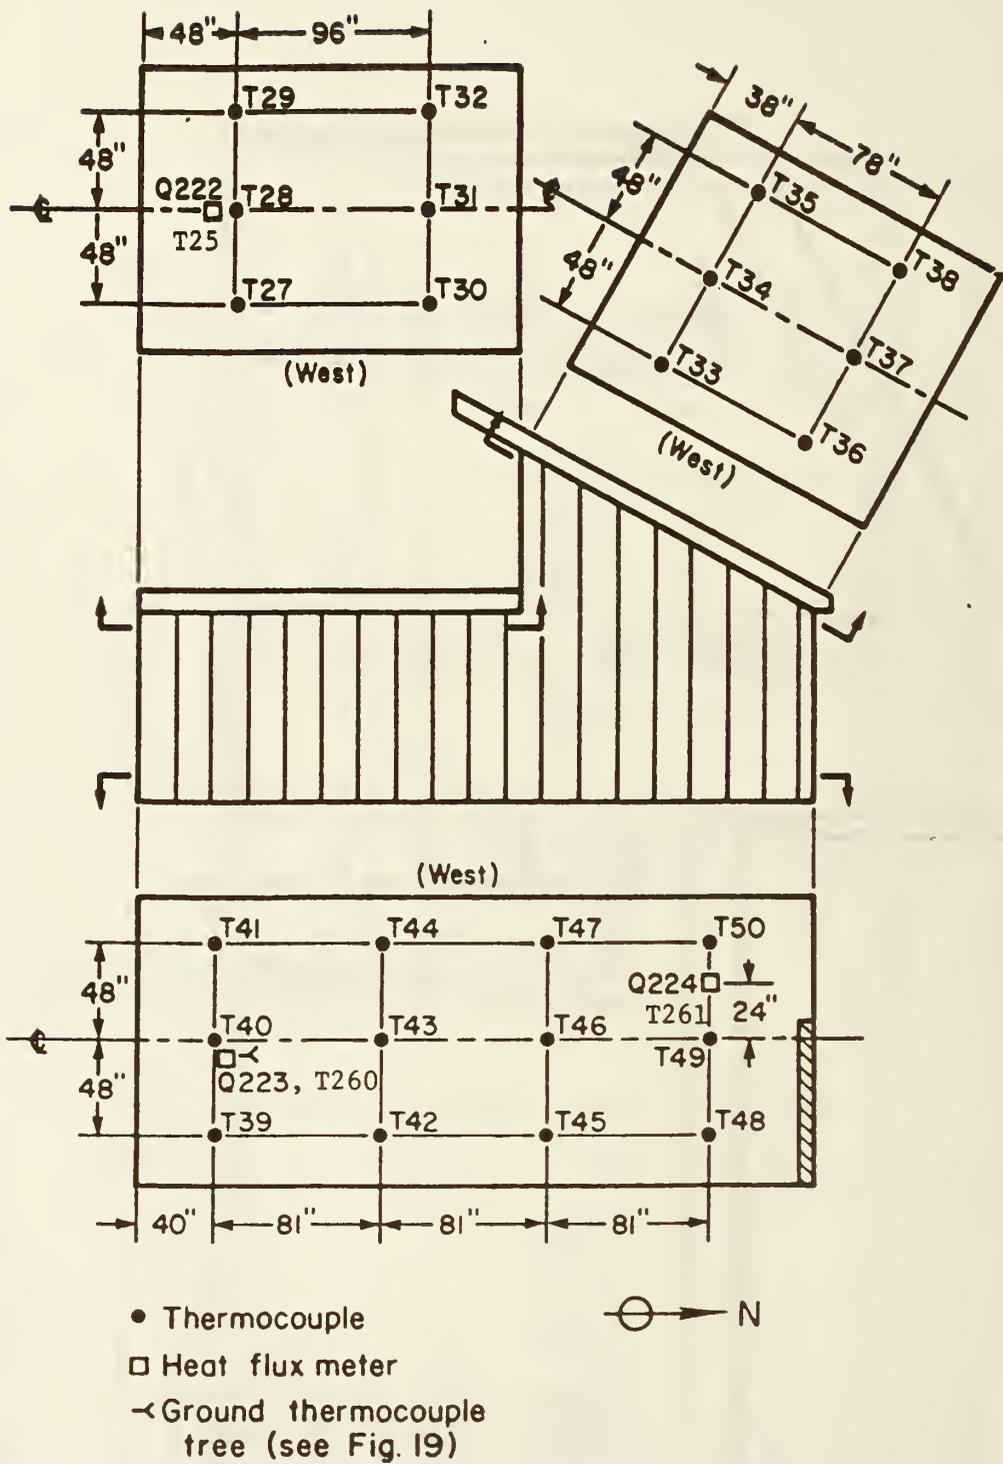


Figure 35. Sensor Locations Ceiling and Floor Cell #4




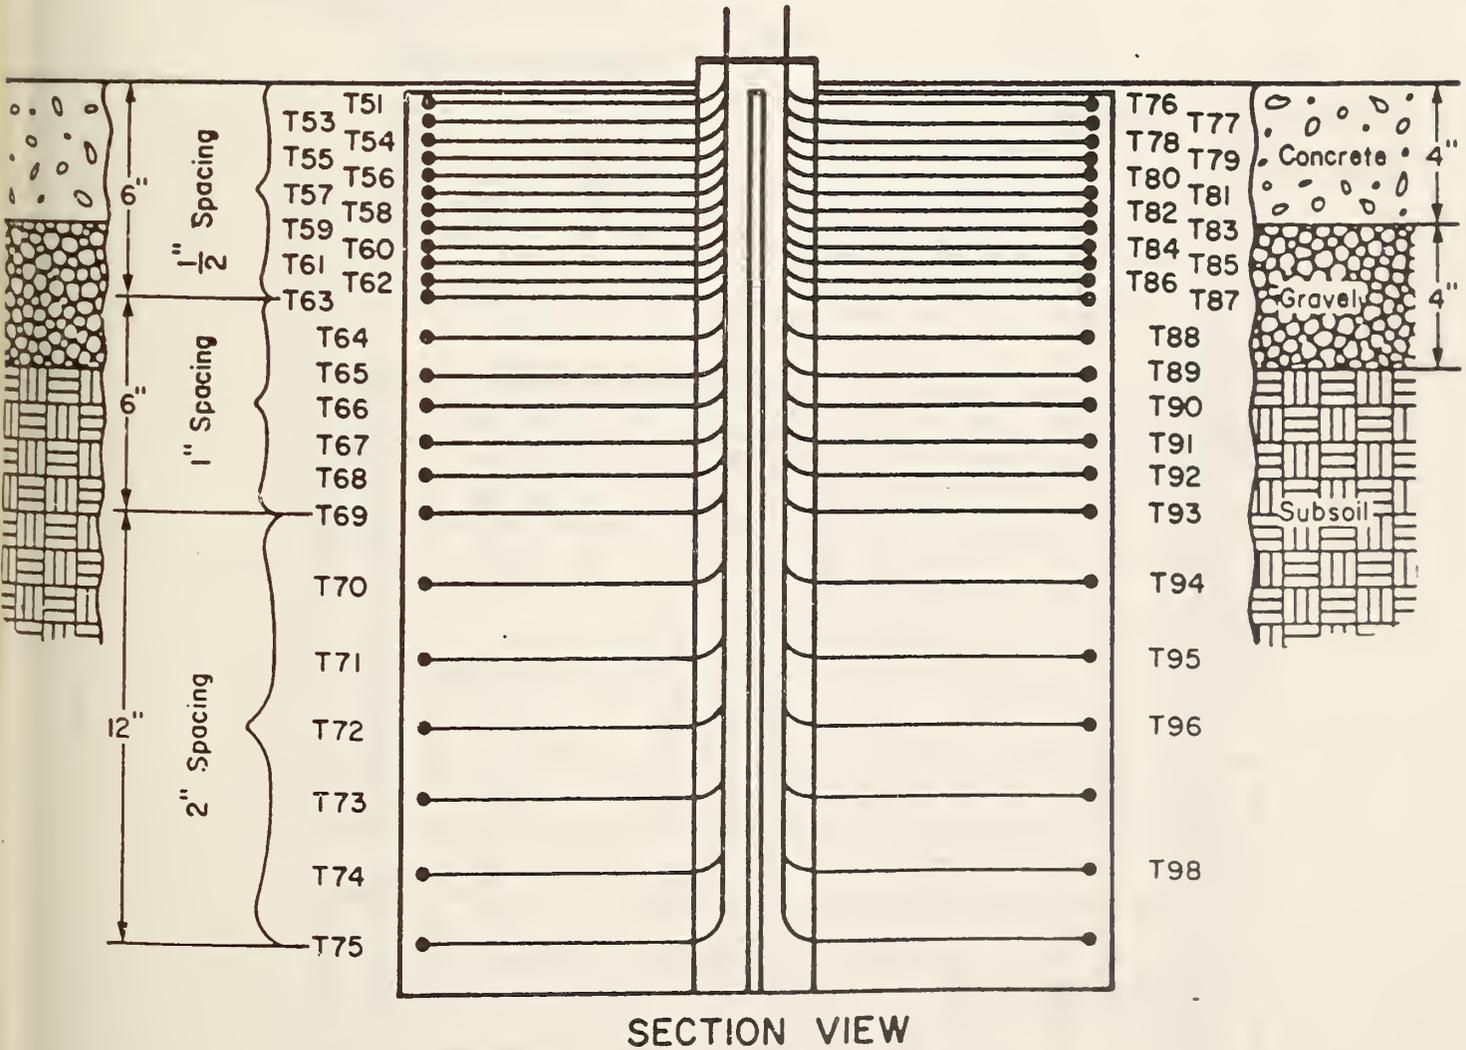


Figure 36. Ground Thermocouple Tree
(See Figure 21 for Location Within Cell #4)

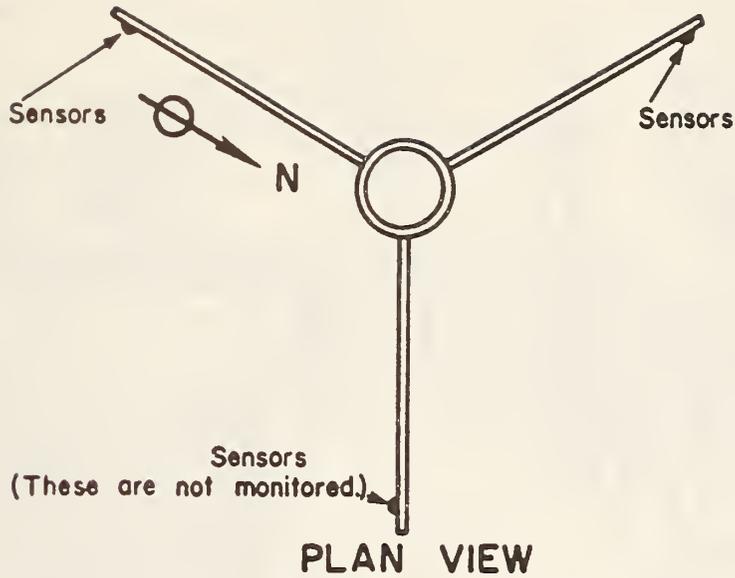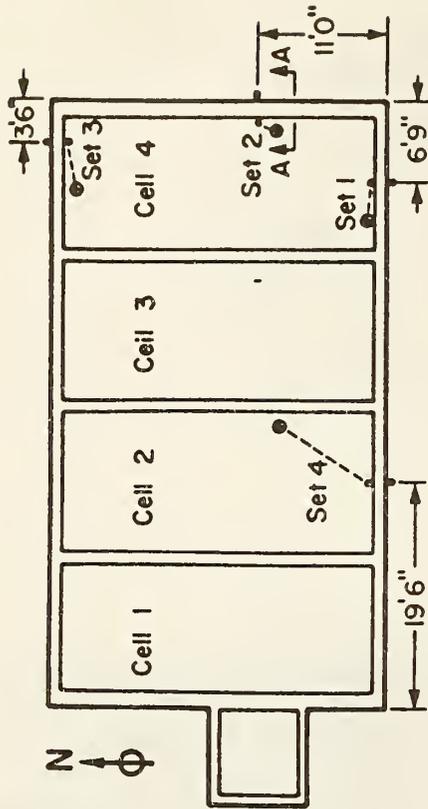

- Standpipe
- Thermocouple String
(Type T₁, #20, teflon coated, etched and coated with thermal epoxy.)

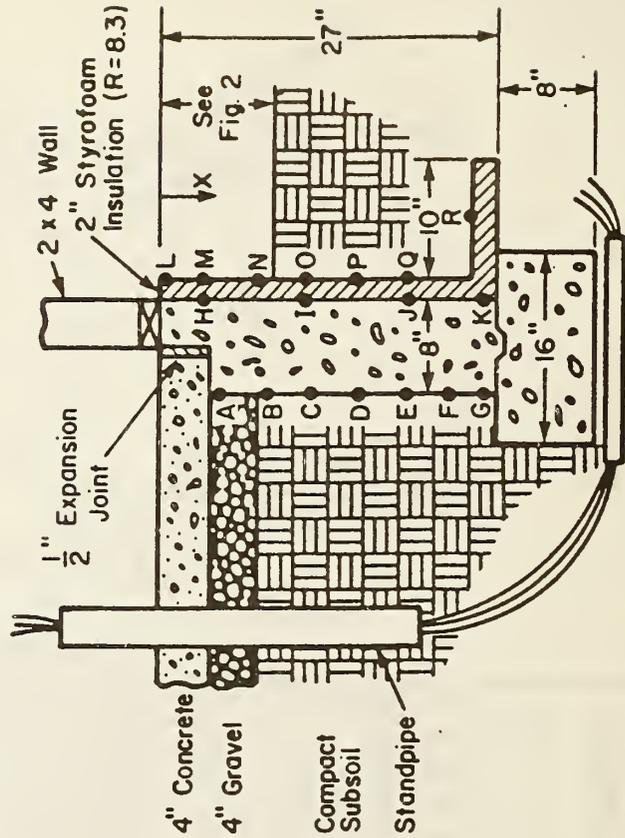

SECTION A-A, TYPICAL

	Set 1		Set 2		Set 3		Set 4	
	X in	Sensor	X cm	X in	Sensor	X cm	X in	Sensor
A	10.8	T101	11.4	4½	T119	12.7	5	T137
B	19.7	T102	21.0	8¼	T120	20.3	8	T138
C	30.5	T103	31.0	12¾	T121	32.4	12¾	T139
D	41.3	T104	41.3	16¾	T122	40.6	16	T140
E	50.8	T105	52.1	20¾	T123	49.5	19½	T141
F	62.2	T106	60.3	23¾	T124	60.3	23¾	T142
G	67.9	T107	68.6	27	T125	69.9	27½	T143
H	12.7	5	10.2	4	T126	10.2	4	T144
I	30.5	12	29.8	11¾	T127	30.5	12	T145
J	50.8	20	49.5	19½	T128	50.8	20	T146
K	67.9	26¾	68.6	27	T129	69.2	27¾	T147
L	1.3	½	1.3	½	T130	1.3	½	T148
M	10.2	4	10.2	4	T131	10.2	4	T149
N	20.3	8	20.3	8	T132	20.3	8	T150
O	30.5	12	30.5	12	T133	30.5	12	T151
P	40.6	16	40.6	16	T134	40.6	16	T152
Q	50.8	20	50.8	20	T135	50.8	20	T153
R	61.0	24	61.0	24	T136	61.0	24	T154

Figure 37. Foundation Temperature Sensor Locations

● Thermocouple (on inside block surface)

□ Heat flux meter

◇ Thermocouples spaced in mortar (T164-T170)

Depth from inside surface	cm	0.32	2.22	6.03	9.84	13.65	17.46	19.05
	inch	0.13	0.88	2.38	3.88	5.38	6.88	7.50
Sensor Number		T164	T165	T166	T167	T168	T169	T170

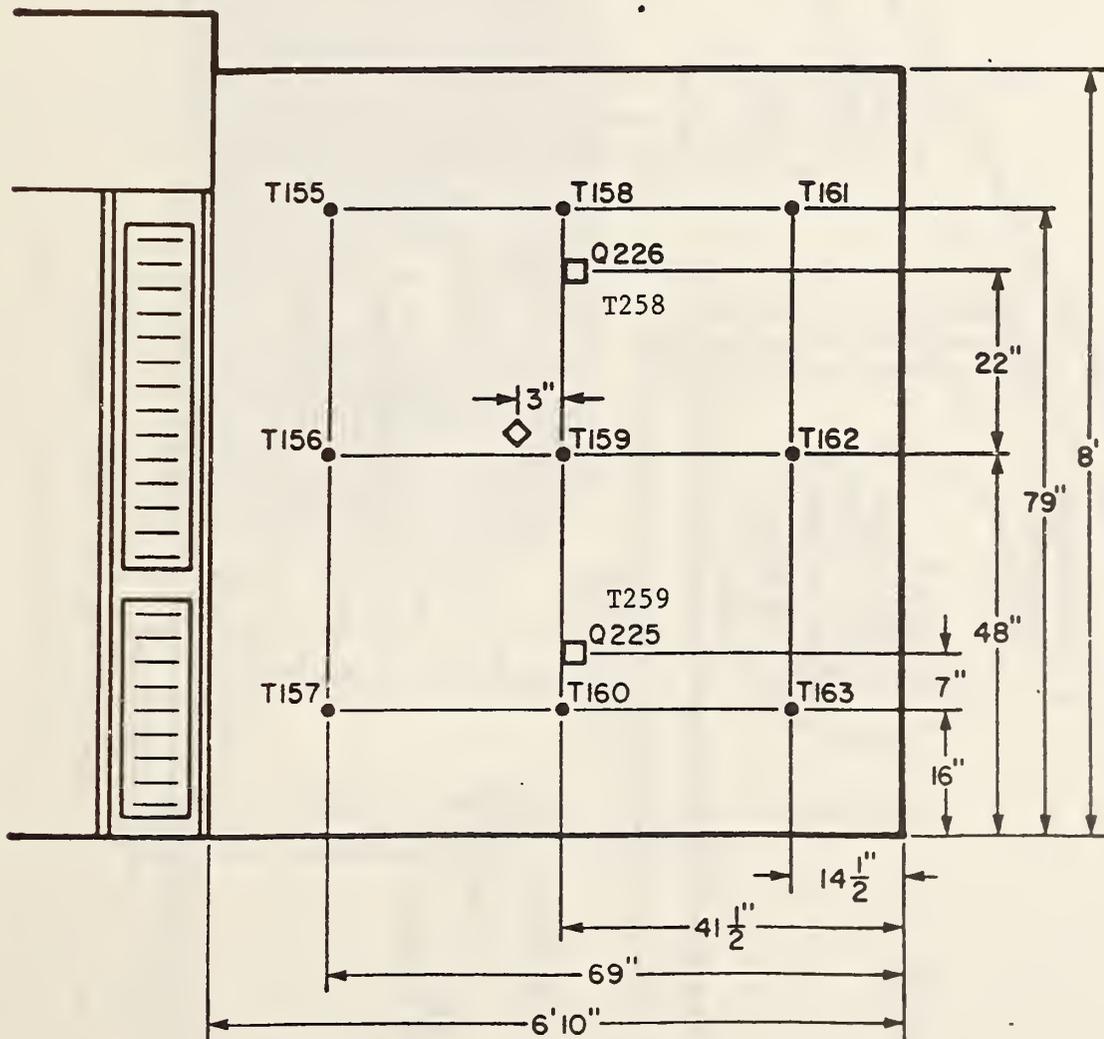


Figure 38. Thermal Storage Wall Sensor Locations in Cell #4

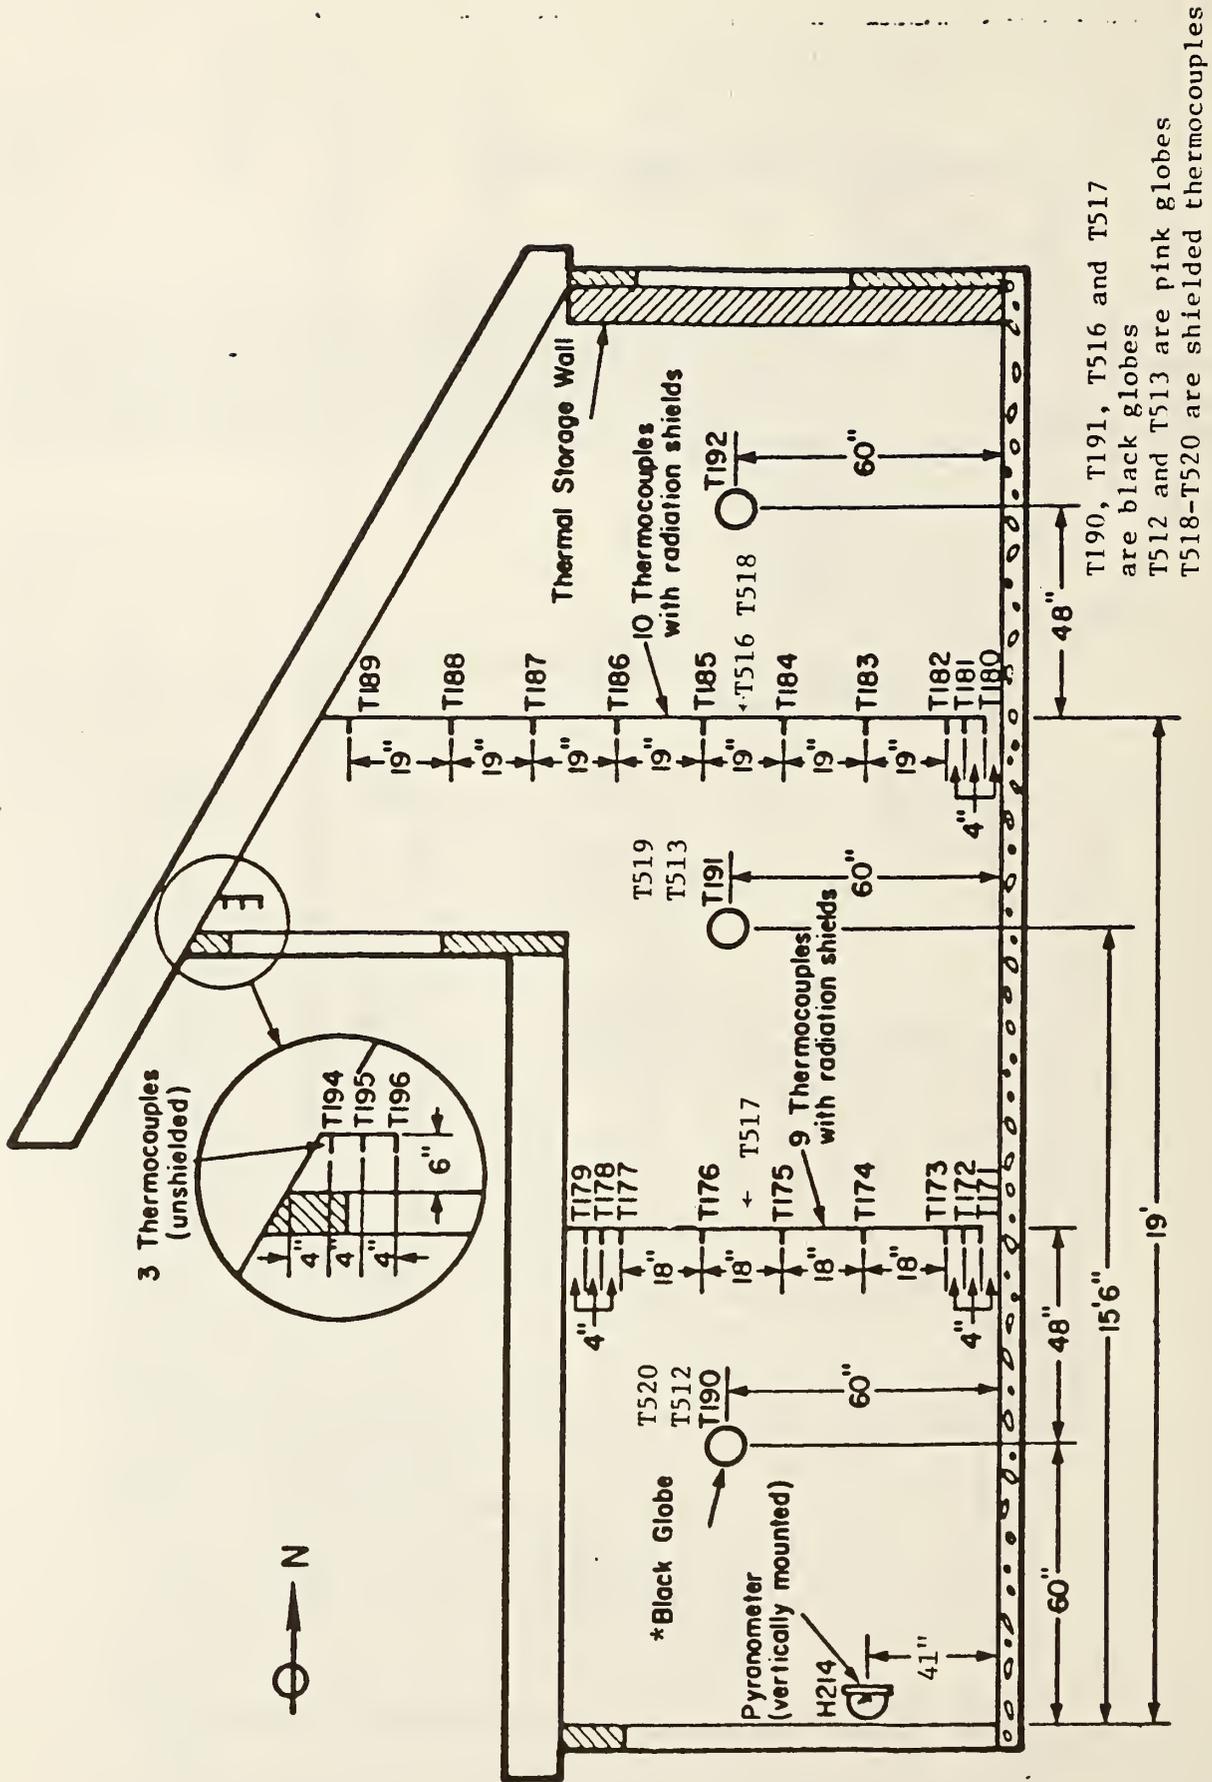


Figure 39. Air Temperature Sensor Locations Cell #4

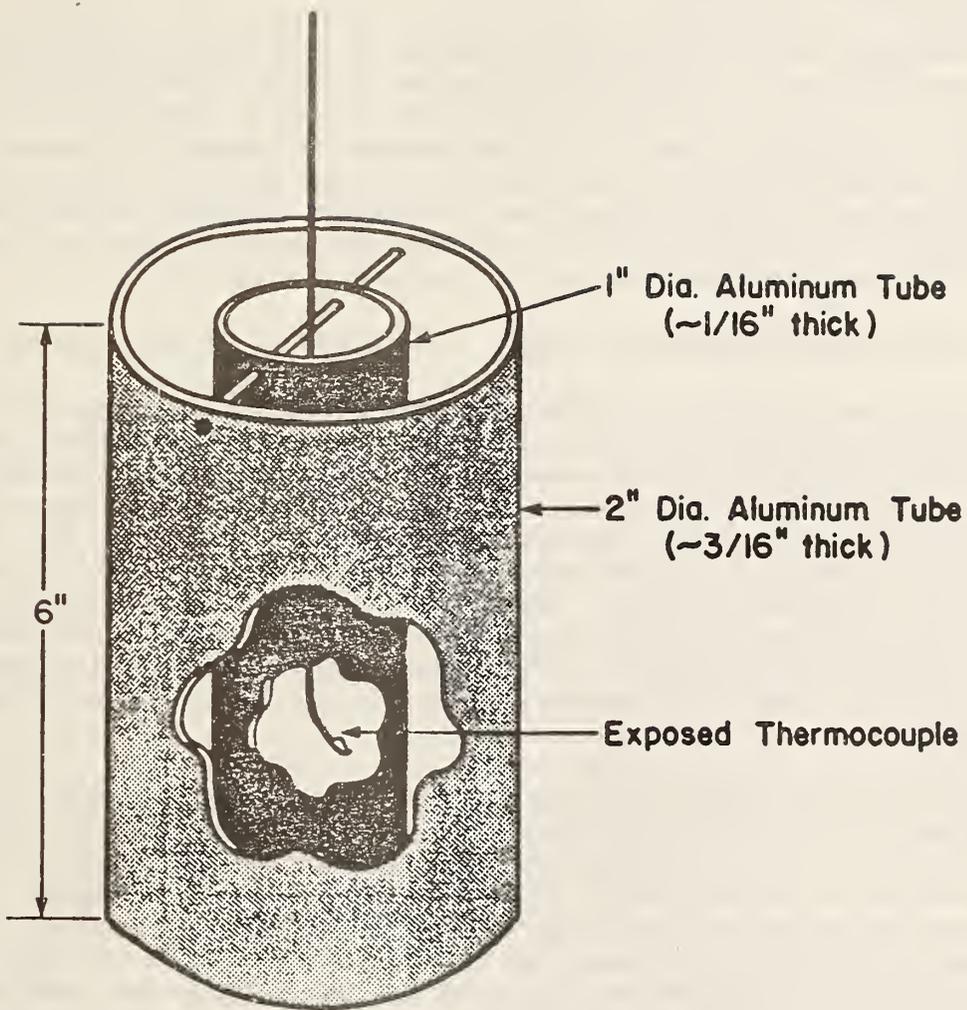


Figure 40. Radiation Shields Used for Thermocouples Measuring Air Temperatures

5. DATA ACQUISITION

5.1 DATA ACQUISITION SYSTEM

The new data acquisition system (DAS) consists of a desktop computer with 575K bytes of memory, a real time clock, and a scanner with an integrating digital voltmeter having one microvolt resolution. This system provides greater capacity and improved reliability than the original system. Currently, the DAS is capable of handling about 500 data channels and its capacity can be expanded to handle 700 channels. The system has two cassette drives, and a 9-track, 1600 BPI magnetic tape drive for data and software storage. The DAS was received in March 1983, and its installation was completed in May 1983.

5.2 AIR INFILTRATION MONITORING SYSTEM

The multi-zone automated air infiltration monitoring system using the tracer gas decay method was designed and built by Dr. Richard Grot of NBS. The system consists of: a S-100 bus microcomputer with two 8-inch floppy disc drives; a real time clock; a CRT terminal; an electron capture gas chromatograph detector which measures the sulfur hexafluoride (SF_6) tracer gas in parts per billion range with an accuracy of 2.5 percent; a ten port sample manifold; a group of five tracer gas injection units; a bank of ten auxiliary sample pumps; input data terminals for the wind speed and direction and the ambient and indoor zone temperatures; and the associated software which monitor and control the operation of the system. A detailed description of the system is contained in reference [8].

The tracer gas decay method was used: it consists of a single injection followed by the measuring of the concentration decay of the tracer gas over a three-hour period. The amount of tracer gas injection through each of the five injection units is determined and controlled independently by the microcomputer on the basis of the concentration decay history of the individual injection zones. Ten sampling locations can be selected within a maximum of five zones. A small amount of the air drawn by the auxiliary sample pumps from the ten locations is fed to the gas chromatograph-detector sequentially for measuring of the tracer gas concentration at the ten locations. Extra-pure argon gas (Ar) is used to flush out the detector system between samples. A one-minute time interval is required for measuring each of the sample concentrations and flushing the detector system after the measurement, resulting in a sampling interval of ten minutes for all ten sampling ports. Therefore, five concentration data points per hour for each of the sampling locations are obtained (the last ten-minute interval is reserved for writing data onto the floppy disc, and injection of tracer gas if necessary). These five data points are used to determine the air infiltration rate in terms of air changes per hour on the basis of tracer decay theory and the least-square technique. Since all the ten-minute concentration data are stored on the floppy disc, more accurate least-square analysis based on 15 data points over a three-hour interval (between injections of tracer gas) can also be performed later if necessary. At present, insufficient data exist for purposes of precision and accuracy determination. A reasonable estimate of the uncertainty in a given air change rate determination is of the order of 10 percent or less [9].

For the present passive solar test house, only three of the five injection units and nine of the ten sampling ports are used. An injection unit with three sampling ports serves each cell. In each cell the injection port is located at the outlet of the fan-coil unit with the fan running continuously to obtain a uniform mixing of the injected tracer gas within the test cell. The three sampling ports within each cell are located at the south, center, and north side of the cell midway between the floor and the ceiling at each location. For the first series of experiments the doors between the cells are kept closed and any opening through the walls between the cells is sealed to prevent air movement between the cells. Infiltration data for each sampling location are computed individually on an hourly basis and the averaged value of the three locations is computed to be the infiltration data for the test cell.

5.3 DATA ACQUISITION AND DISTRIBUTION

With the exception of air infiltration data which is on a separate system, all data are taken by the new data acquisition system and stored on the magnetic tape. The solar radiation and weather data are taken at one-minute intervals, watt-hour data are taken at one-hour intervals, and all other data are taken at ten-minute intervals. These data are later numerically integrated and averaged to create hourly average data sets. The hourly average data sets including hourly air infiltration data are recorded onto a magnetic tape in a prior agreed format. A documentation file containing the test conditions and an index to the data records is also recorded onto the magnetic tape. A printout of the "Data Documentation" is given in Appendix A as an example. The data tape along with a printout of the documentation is distributed to the participant researchers for their use. The hourly average data sets are also archived at the National Bureau of Standards from where they are available upon request.

5.4 ESTIMATES OF UNCERTAINTY IN THE MEASURED DATA

Some of the factors that contribute to the uncertainty in the measured data include type of measurement or data, type of sensor used and the material of its construction, application environment and sensor mounting techniques, data scanning and logging equipment, and conversion from electrical signals of sensors to engineering quantities. Estimates of measurement uncertainty for various types of data taken at the NBS test facility are given in table 6, and are discussed below:

Table 4. Estimates of Measurement Uncertainty for Different Data

Item #	Data Type	Estimated Measurement Uncertainty
1	Air infiltration	+ 10%
2	Auxiliary energy	< 0.1%
3	Heat flux	currently indeterminate
4	Solar radiation	+ 5.0%
5	Temperature	+ 0.5°C
6	Wind speed	+ 2.0% with threshold 0.58 m/s
	Wind direction	+ 3 degrees

Air Infiltration

It was discussed earlier in the previous section that at the present state-of-the-art the existing data are insufficient for the purposes of precision and uncertainty determination. A reasonable estimate of uncertainty in a given air change rate, measured by the tracer gas decay method, is about + 10 percent [9].

Auxiliary Energy Supply

The auxiliary energy supplied to the three test cells via six watt-hour meters is measured by a six pulse counter with the minimum interval equal to 1.8 watt-hours. Therefore, regardless of the measurement interval the maximum uncertainty of + 1.8 watt-hour is expected in a given measurement. The long term uncertainty in the energy supply measurement is estimated to be less than + 0.1 percent by repeated comparison of measured data with commercial watt-hour meter readings.

Heat Flux

The heat-flux meter used in the direct gain cell (i.e., cell #4) of the NBS test facility were calibrated in a sandwich mode using the "guarded hot-plate" facility at NBS. However, a definitive estimate of uncertainty in the measured heat flux data cannot be made at present.

The measurement of heat flux with heat flow sensor (heat-flux meter) was the subject of a two-day workshop sponsored by the American Society for Testing and Materials (ASTM). The author attended the ASTM Workshop on Building Application of Heat Flow Sensors held at the ASTM headquarters in Philadelphia, PA, on September 22-23, 1983. The general opinion of the experts in the field is that the measurements of heat flow with heat-flux meters are not very reliable, particularly if the meter's application condition are not similar to the meter's calibration condition. Also, presently the techniques or the procedures for calibrating a heat-flux meter are not standardized.

Some of the factors which contribute to uncertainty of heat flow measurement include: (1) thermal and radiometric properties of the meter material with respect to those of the test structure material; (2) contact resistance due to contact between the meter and test article; (3) convection around the meter; (4) multidimensional conduction; (5) thermal inertia of meter with respect to that of the test structure; and (6) instability of heat field or unsteady nature of heat transfer process [10]. More experimental research is needed to quantify the effects of the abovementioned factors on the heat flow data measured by heat-flux meters.

Solar Radiation

Solar radiometry is an inexact science with international comparisons showing disagreement of as much as 7 percent [11]. The sensitivity of Normal Incident Pyrheliometers (NIP's) is in general shown to be within 0.5 percent of absolute cavity radiometers that defines the World's Radiometric Reference Scale [12,13]. The NIP used at the test facility has been calibrated within the year and intercompared within 1 percent to other NIPs. Since the NIP readings are sensitive to the alignment, the tracer of the NIP is realigned twice a day for the duration of each tests at the NBS test facility.

A sensitivity intercomparison of four side-by-side PSP pyrometers showed an agreement of within 1 percent [14]. In this intercomparison the temperature correction was not made and cosine response was not determined. Instantaneous values may be uncertain by as much as 3 percent depending on conditions. The instruments used at the NBS test facility are by one manufacturer and are periodically recalibrated by the supplier. Also, these instruments have been periodically intercompared at the test facility and the data agreed within 1 percent. Some uncertainty in the pyrometer data may also arise due to misalignment of the instrument. A conservative estimate of overall uncertainty in the solar radiation data is ± 5 percent.

Temperatures

The thermocouples at the NBS test facility were installed by following the "procedures for minimizing error" described in the ASTM Special Technical Publication, ASTM SPT-470 [15]. Some of the thermocouples, before their installation were calibrated in standard ice and hot water baths by following the procedures described in the ASTM Standard E-220-80 [14]. These thermocouples were calibrated over the temperature range of 0.0 to 60°C, and thermocouple data were within $\pm 0.2^\circ\text{C}$ of the reading of the standard thermometer. The voltage data from thermocouples are converted to temperatures in degree Celsius ($^\circ\text{C}$) by using the quadratic expansion equation and the values of expansion coefficients given in reference 17. The uncertainty due to long leads of the thermocouples is considered to be negligible. Additional unknown uncertainties due to inhomogeneity and change in material properties is anticipated.

The thermocouples used for measuring the room air temperature in cells #2 and #4 are provided with double radiation shields (see figure 40). The effectiveness of the shields were tested at NBS as: the data from shielded thermocouples were compared with data from mechanically aspirated and shielded

thermocouples the readings were within $\pm 0.1^\circ$ of each other. An estimate of the maximum overall uncertainty in the thermocouples data, including errors due to reference, multiplexing, and conversion, is $\pm 0.5^\circ\text{C}$.

Wind Speed and Direction

The anemometer and vane used for measuring the wind speed is factory calibrated and has a claimed uncertainty of ± 2 percent with a threshold of 0.58 m/s; and wind direction is ± 3 degrees.

Data Scanner

For verifying the resolution of the digital voltmeter of the data scanner and for assuring that the DAS is functioning properly, the DAS is provided with one reference, one millivolt signal, and five reference zero volt signals. The zero volt signals are produced by electrically shorting a data channel on a multiplexing card. The reference signals are placed on five different strategically selected multiplexing cards. The one millivolt reference channel and one of the reference zero volt channel are scanned at one-minute intervals, and all of the six reference voltage channels are scanned at ten-minute intervals. The one-minute interval data are only displayed on the CRT (screen), while the ten-minute interval data from these reference channels in addition to being displayed on the CRT is also recorded on the magnetic tape along with other data. The data taken to-date has assured us that the system had been functioning properly during the experiments, and has also verified the acclaimed 1 microvolt resolution of the voltmeter.

6. CONCLUDING REMARKS

As a part of the DoE's Experimental Systems Research Program, the NBS Passive Solar Test facility has been constructed in Gaithersburg, Maryland. The test facility is used to collect class A level performance monitoring data for different passive solar system under different experimental conditions. The data is distributed to various researchers for use in: (1) detailed building energy analysis and models/algorithms validation; and (2) performance characterization of passive solar systems. This handbook provides, for the users of these data (i.e., models/algorithms developers/validators), a complete physical description of the test building, sensor locations, data acquisition procedures, and an estimate of uncertainty in the measured data.

The following items are available from the National Bureau of Standards: (1) This handbook; (2) data documentation (see appendix); and (3) magnetic tapes containing hourly average sets of data collected at the NBS test facility. Additional information concerning the NBS Passive Solar Test Facility and Experimental Data may be obtained from:

Bal Mahajan
Building Equipment Group/Building Equipment Division
Center for Building Technology
National Bureau of Standards/Building 226/ Room B306
Washington, D.C. 20234
Phone (301)-921-3294

7. ACKNOWLEDGEMENT

This work is sponsored by the Passive and Hybrid Solar Division, Office of Solar Heat Technologies, U.S. Department of Energy, Washington, DC 20585, as part of the experimental system research program.

The author wishes to express his sincere gratitude to Dr. Kent A. Reed and Dr. Stanley T. Liu for their many valuable suggestions.

8. REFERENCE

1. "Program Area Plan: Performance Evaluation of Passive/Hybrid Solar Heating and Cooling Systems," Solar Energy Research Institute Report SERI/PR-721-788, October 1980, Golden, CO.
2. Hamilton, B. L. and Scofield, P. M., "National Passive/Hybrid Performance Evaluation Program for System Development," Proceedings of the 5th National Passive Solar Conference, Amherst, MA, October 1980.
3. Lindler, Keith W., "National Bureau of Standards Passive Solar Test Building Handbook," NBS-GCR-82-398, August 1982, National Bureau of Standards Washington, DC 20234.
4. Mahajan, Bal M. and Liu, Stanley T., "Initial Results from the NBS Passive Solar Test Facility," Proceedings of the ASME Solar Division Sixth Annual Technical Conference, April 19-21, 1983
5. Mahajan, Bal M. and Liu Stanley T., "Results from the NBS Passive Test Facility - A Status Report," Proceedings of the Passive and Hybrid Solar Energy Update, September 26-28, 1983.
6. McCabe, M. E., Bushby, S., and Ducas, W., "Conceptual Design and Performance Specification for the Passive Solar Component Calorimeter," NBS Letter Report to DoE, March 1982.
7. "National Bureau of Standards Direct-Gain Test Cell Site Handbook," Los Alamos National Laboratory Report No. LA-9786-MS, edited by Nancy Sheheen, Q Division, 1983.
8. Grot, R. A., Hunt, C. M., and Harrje, D. T., "Automatic Air Infiltration Measurements in Large Buildings," Proceeding of the First AIC Conference Infiltration and Measuring Techniques; Windsor, U. K., October 8-10, 1980.
9. ASTM Standard E741.80, "Standard Practice for Measuring Air Leakage Rate Using Tracer Dilution Method," ASTM, 1980.
10. Johannesson, Gudni., "Heat Flow Measurements: Thermoelectrical Meters, Function Principles and Sources of Errors," Lund Institute of Technology Report TVBH-3003, Lund, Sweden, 1979. Translated by U.S. Army Corps of Engineering, March 1982.
11. Proceedings of the International Energy Agency Conference on Pyronometer Measurements, Final Report," SERI/TR-642-1156R, March 1981, Solar Energy Research Institute, Boulder, CO.
12. Zerlant, G. A., Bern, J., Maybee, J., and Nooring, W., "The 1981 Intercomparison of Pyronometers and Normal Incident Beam Pyrheliometers at New River, Arizona, I. Pyrheliometers," DSET Report 81-1218L, December 1981.

13. Zerlaut, G. A., Bern, J., Maybee, J., and Nooring, W., "The Second New River Intercomparison of Pyronometers and Normal Beam Pyrheliometers," DSET Report 82-0703E, July 1982.
14. Zerlaut, G. A., Bern, J., Maybee, J., and Nooring, W., "The 1981 Intercomparison of Pyronometers and Normal Incident Pyrheliometers at New River, Arizona. II. Pyronometers," DSET Report 82-0104L, January 4, 1982.
15. "Manual on the Use of Thermocouples in Temperature Measurement," ASTM Special Technical Publication, ASTM STP-470, 1980.
16. ASTM, "Calibration of Thermocouples by Comparison," ASTM Standard E228-80; 1980.
17. Powel, R. L. et al., "Thermocouples Reference Tables Based on the JPTS-68;" NBS Monograph 125, March 1974.

APPENDIX A

A copy of the "Data Documentation" distribution to various researchers along with the data tapes.

DATA DOCUMENTATION.

THE ACCOMPANYING MAGNETIC TAPE CONTAINS DATA COLLECTED AT THE NATIONAL BUREAU OF STANDARDS PASSIVE SOLAR TEST FACILITY DURING TESTS CONDUCTED FROM FEBRUARY 17, 1984 TO MARCH 12, 1984.

CONDITIONS FOR THE TESTS WERE:

LOWER BOUND TEMPERATURE: FIXED IN ALL CELLS.

UPPER BOUND TEMPERATURE: FREE FLOATING IN ALL CELLS.

CLERESTORY SHUTTERS: CLOSED IN CELL #3. & OPEN IN CELLS #2 & #4.

VENTS OF THE TROMBE WALL: BLOCKED IN CELL #2.

FAN COIL UNIT FAN: ON IN ALL CELLS.

ADDITIONAL DESTRATIFYING FANS: ON IN CELL #4.

THE TAPE'S CONTENTS ARE:

- 1) DOCUMENTATION FILE (THE MATERIAL YOU ARE READING).
- 2) EOF
- 3) DATA FILE FROM 2/17, HOUR 16 TO 3/12, HOUR 16
- 4) EOF
- 5) EOF

THE DATA FILES ARE ARRANGED INTO ROWS AND COLUMNS WITH EACH ROW CORRESPONDING TO A LOGICAL RECORD ON THE MAGNETIC TAPE AND EACH COLUMN CORRESPONDING TO AN ENTRY IN THE RECORD. THE FIRST ENTRY IN EACH RECORD IS THE NUMBER OF THE ROW TO WHICH THE RECORD CORRESPONDS. WHILE THE FOLLOWING EIGHT ENTRIES IN THE RECORD REPRESENT THE HOURLY AVERAGE READINGS. EACH SET OF 56 ROWS CONSTITUTES A PHYSICAL BLOCK ON THE MAGNETIC TAPE. EACH PHYSICAL BLOCK CONTAINS A COMPLETE SET OF HOURLY AVERAGE READINGS FOR A GIVEN HOUR , FOR THE SENSORS MONITORED AT THE PASSIVE TEST FACILITY.

THE READINGS FOR THE AVERAGES WERE TAKEN AS FOLLOWS

EVERY HOUR - AUXILIARY ENERGY SUPPLIED AND AIR INFILTRATION.

EVERY 1 MINUTE - WIND SPEED AND DIRECTION. AND SOLAR RADIATION.

EVERY 10 MINUTES - ALL OTHER READINGS.

THE DATA ARE WRITTEN WITH THE FOLLOWING SPECIFICATIONS

FORMAT.....(I2.8F9.2)

CHARACTER SET.....ASCII

TAPE DENSITY.....1600 BPI

TRACKS.....9

CHARACTERS/RECORD.....80

RECORDS/BLOCK.....56

ALL TIMES REFER TO EASTERN STANDARD TIME.

AN INDEX TO THE DATA IS GIVEN BELOW.

LOCATION/DESCRIPTION OF EACH SENSOR IS FOLLOWED BY A LABEL. THE LABEL IN THE PARENTHESIS IS SAME AS THE LABEL IN THE SITE HANDBOOK.

THE SENSORS ARE LABELED BY A LETTER AND A NUMBER. THE LETTERS INCLUDE H(RADIATION), Q(HEAT FLUX), T(TEMPERATURE), W(WEATHER), AND WH(WATT-HOUR). ALL TEMPERATURES, UNLESS SPECIFIED OTHERWISE, ARE MEASURED WITH TYPE T THERMOCOUPLES.

HEAT FLUX AND RADIATION DATA ARE GIVEN AS W/M^2 , TEMPERATURES IN DEGREE C, UXILIARY ENERGY IN WATT-HOURS , WIND SPEED IN M/S . AND WIND DIRECTION IN DEGREES.

AN ASTERISK INDICATES THAT THE SENSOR WAS INOPERATIVE OR WAS NOT MONITORED, AND A VALUE OF 9999.99 IS GIVEN AS DATA FOR THE SENSOR.

ANY QUESTIONS REGARDING THIS DATA SHOULD BE ADDRESSED TO

BAL M. MAHAJAN / STANLEY T. LIU

BLDG 226 . ROOM B306

CENTER FOR BUILDING TECHNOLOGY

NATIONAL BUREAU OF STANDARDS

WASHINGTON D.C. 20234

PHONE 301-921-3294 OR 301-921-2607 (COMMERCIAL)

921-3294 OR 921-2607 (FTS)

.....

ROW 1

COLUMN		
1	YEAR	
2	DAY	
3	HOUR	
4	REFERENCE MILLIVOLT SIGNAL	
5	REFERENCE ZERO	
6	NOT USED	(9999.99)
7	NOT USED	(9999.99)
8	NOT USED	(9999.99)

ROW 2

COLUMN		
1	VERTICAL RADIATION BEHIND GLASS CELL 4	(H214)
2	VERTICAL RADIATION OUTSIDE OF GLASS CELL 4	(H215)
3	SKY INFRARED RADIATION	(H216)
4	TOTAL HORIZONTAL RADIATION (ON ROOF)	(H217)
5	GROUND REFLECTED RADIATION	(H218)
6	DIRECT NORMAL RADIATION	(H219)
7	WIND SPEED (M/S)	(W1)
8	WIND DIRECTION ANGLE (DEGREES) MEASURED CLOCKWISE FROM NORTH	(W2)

ROW 3

COLUMN		
1	HEAT FLUX BHND EAST WALL 163 CM FRM SOUTH WALL 136 CM FROM FLOOR CELL #4	(Q220)
2	HEAT FLUX AS ABOVE. BUT ON SURFACE OF E WALL	(Q221)
3	HEAT FLUX LEVEL CEIL 187 CM FRM WEST WALL 111 CM FROM SOUTH WALL CELL #4	(Q222)
4	HEAT FLUX FLOOR. SOUTH SECT. 200 CM FRM WEST WALL 119 CM FRM SOUTH WALL CELL #4	(Q223)
5	HEAT FLUX FLOOR. NORTH SECT. 731 CM FRM SOUTH WALL 124 CM FROM WEST WALL CELL #4	(Q224)
6	HEAT FLUX STRG WALL BOT. 268 CM FRM WEST WALL 57 CM FROM FLOOR CELL #4	(Q225)
7	HEAT FLUX STRG WALL TOP. 268 CM FRM WEST WALL 178 CM FROM FLOOR CELL #4	(Q226)
* 8	HEAT FLUX BHND EAST WALL. 613 CM FRM SOUTH WALL 139 CM FROM FLOOR CELL #4	(Q227)

ROW 4

COLUMN		
1	HEAT FLUX AS ABOVE. BUT ON SURFACE OF E WALL	(Q228)
2	HEAT FLUX SURFACE EAST WALL 314 CM FRM SOUTH WALL 142 CM FROM FLOOR CELL #4	(Q229)
* 3	HEAT FLUX SURFACE EAST WALL 712 CM FR SOUTH WALL 142 CM FR FLOOR CELL #4	(Q230)
4	RTD CELL #2 FCU IN	(R231)
5	RTD CELL #2 FCU OUT	(R232)
6	RTD CELL #3 FCU IN	(R233)
7	RTD CELL #3 FCU OUT	(R234)
* 8	RTD CELL #4 FCU IN	(R235)

ROW 5

COLUMN

1	RTD CELL #4 FCU OUT	(R236)
* 2	RTD CELL #4 499 CM FR SOUTH WALL 150 CM FR FLOOR NEAR THERMOSTAT	(R237)
3	E WALL SURF TEMP CELL #4 122 CM FROM S WALL 41 CM FRM FLOOR	(T1)
4	E WALL SURF TEMP CELL #4 122 CM FROM S WALL 122 CM FRM FLOOR	(T2)
5	E WALL SURF TEMP CELL #4 122 CM FROM S WALL 203 CM FRM FLOOR	(T3)
6	E WALL SURF TEMP CELL #4 366 CM FROM S WALL 41 CM FRM FLOOR	(T4)
7	E WALL SURF TEMP CELL #4 366 CM FROM S WALL 122 CM FRM FLOOR	(T5)
8	E WALL SURF TEMP CELL #4 366 CM FROM S WALL 203 CM FRM FLOOR	(T6)

ROW 6

COLUMN

1	E WALL SURF TEMP CELL #4 533 CM FROM S WALL 51 CM FRM FLOOR	(T7)
2	E WALL SURF TEMP CELL #4 533 CM FROM S WALL 150 CM FRM FLOOR	(T8)
3	E WALL SURF TEMP CELL #4 533 CM FROM S WALL 249 CM FRM FLOOR	(T9)
4	E WALL SURF TEMP CELL #4 533 CM FROM S WALL 348 CM FRM FLOOR	(T10)
5	E WALL SURF TEMP CELL #4 700 CM FROM S WALL 51 CM FRM FLOOR	(T11)
6	E WALL SURF TEMP CELL #4 700 CM FROM S WALL 152 CM FRM FLOOR	(T12)
7	E WALL SURF TEMP CELL #4 700 CM FROM S WALL 254 CM FRM FLOOR	(T13)
8	W WALL SURF TEMP CELL #4 122 CM FROM S WALL 41 CM FRM FLOOR	(T14)

ROW 7

COLUMN

1	W WALL SURF TEMP CELL #4 122 CM FROM S WALL 122 CM FRM FLOOR	(T15)
2	W WALL SURF TEMP CELL #4 122 CM FROM S WALL 203 CM FRM FLOOR	(T16)
3	W WALL SURF TEMP CELL #4 366 CM FROM S WALL 51 CM FRM FLOOR	(T17)
4	W WALL SURF TEMP CELL #4 366 CM FROM S WALL 152 CM FRM FLOOR	(T18)
5	W WALL SURF TEMP CELL #4 366 CM FROM S WALL 203 CM FRM FLOOR	(T19)
6	W WALL SURF TEMP CELL #4 533 CM FROM S WALL 51 CM FRM FLOOR	(T20)
7	* W WALL SURF TEMP CELL #4 533 CM FROM S WALL 150 CM FRM FLOOR	(T21)
8	W WALL SURF TEMP CELL #4 533 CM FROM S WALL 249 CM FRM FLOOR	(T22)

ROW 8

COLUMN

1	W WALL SURF TEMP CELL #4 533 CM FROM S WALL 348 CM FRM FLOOR	(T23)
2	W WALL SURF TEMP CELL #4 700 CM FROM S WALL 51 CM FRM FLOOR	(T24)
3	W WALL SURF TEMP CELL #4 700 CM FROM S WALL 152 CM FRM FLOOR	(T25)
4	W WALL SURF TEMP CELL #4 700 CM FROM S WALL 254 CM FRM FLOOR	(T26)
5	CEIL SURF TEMP CELL #4 122 CM FRM S WALL 122 CM W OF CENT LN	(T27)
6	CEIL SURF TEMP CELL #4 122 CM FRM S WALL ON CENT LN	(T28)
7	CEIL SURF TEMP CELL #4 122 CM FRM S WALL 122 CM E OF CENT LN	(T29)
8	CEIL SURF TEMP CELL #4 366 CM FRM S WALL 122 CM W OF CENT LN	(T30)

ROW 9

COLUMN

1	CEIL SURF TEMP CELL #4 366 CM FRM S WALL ON CENT LN	(T31)
2	CEIL SURF TEMP CELL #4 366 CM FRM S WALL 122 CM E OF CENT LN	(T32)
3	SLOPED CEIL 97 CM ALONG SURF FR CLRSTY 122 CM W OF CENTER LN	(T33)
4	SLOPED CEIL 97 CM ALONG SURF FR CLRSTY ON CENTER LN	(T34)
5	SLOPED CEIL 97 CM ALONG SURF FR CLRSTY 122 CM E OF CENTER LN	(T35)
6	SLOPED CEIL 290 CM ALONG SURF FR CLRSTY 122 CM W OF CENTER LN	(T36)
7	SLOPED CEIL 290 CM ALONG SURF FR CLRSTY ON CENTER LN	(T37)
8	SLOPED CEIL 290 CM ALONG SURF FR CLRSTY 122 CM E OF CENTER LN	(T38)

ROW 10

COLUMN

1	FLOOR SURF TEMP CELL #4 102 CM FRM S WALL 122 CM E OF CENT LN (T39)
2	FLOOR SURF TEMP CELL #4 102 CM FRM S WALL ON CENT LN (T40)
3	FLOOR SURF TEMP CELL #4 102 CM FRM S WALL 122 CM W OF CENT LN (T41)
4	FLOOR SURF TEMP CELL #4 307 CM FRM S WALL 122 CM E OF CENT LN (T42)
5	FLOOR SURF TEMP CELL #4 307 CM FRM S WALL ON CENT LN (T43)
6	FLOOR SURF TEMP CELL #4 307 CM FRM S WALL 122 CM W OF CENT LN (T44)
7	FLOOR SURF TEMP CELL #4 513 CM FRM S WALL 122 CM E OF CENT LN (T45)
8	FLOOR SURF TEMP CELL #4 513 CM FRM S WALL ON CENT LN (T46)

.....

ROW 11

COLUMN

1	FLOOR SURF TEMP CELL #4 513 CM FRM S WALL 122 CM W OF CENT LN (T47)
2	FLOOR SURF TEMP CELL #4 719 CM FRM S WALL 122 CM E OF CENT LN (T48)
3	FLOOR SURF TEMP CELL #4 719 CM FRM S WALL ON CENT LN (T49)
4	FLOOR SURF TEMP CELL #4 719 CM FRM S WALL 122 CM W OF CENT LN (T50)
5	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 1.3 CM (0.5 INCHES) (T51)
6	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 2.5 CM (1 INCHES) (T53)
7	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 3.8 CM (1.5 INCHES) (T54)
8	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 5.0 CM (2 INCHES) (T55)

.....

ROW 12

COLUMN

1	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 6.4 CM (2.5 INCHES) (T56)
2	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 7.6 CM (3 INCHES) (T57)
3	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 8.9 CM (3.5 INCHES) (T58)
4	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 10.2 CM (4 INCHES) (T59)
5	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 11.4 CM (4.5 INCHES) (T60)
6	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 12.7 CM (5 INCHES) (T61)
7	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 14.0 CM (5.5 INCHES) (T62)
8	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 15.2 CM (6 INCHES) (T63)

.....

ROW 13

COLUMN

1	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 17.8 CM (7 INCHES) (T64)
2	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 20.3 CM (8 INCHES) (T65)
3	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 22.9 CM (9 INCHES) (T66)
4	* FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 25.4 CM (10 INCHES) (T67)
5	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 27.9 CM (11 INCHES) (T68)
6	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 30.5 CM (12 INCHES) (T69)
7	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 35.6 CM (14 INCHES) (T70)
8	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 40.6 CM (16 INCHES) (T71)

.....

ROW 14

COLUMN

1	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 45.7 CM (18 INCHES) (T72)
2	* FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 50.8 CM (20 INCHES) (T73)
3	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 55.9 CM (22 INCHES) (T74)
4	FLOOR TEMP CELL #4 PROBE #2 (SOUTH) AT 61.0 CM (24 INCHES) (T75)
5	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 1.3 CM (0.5 INCHES) (T76)
6	* FLOOR TEMP CELL #4 PROBE #3 (NW) AT 2.5 CM (1 INCHES) (T77)
7	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 3.8 CM (1.5 INCHES) (T78)
8	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 5.0 CM (2 INCHES) (T79)

.....

ROW 15

COLUMN

1	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 6.4 CM (2.5 INCHES)	(T80)
2	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 7.6 CM (3 INCHES)	(T81)
3	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 8.9 CM (3.5 INCHES)	(T82)
4	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 10.2 CM (4 INCHES)	(T83)
5	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 11.4 CM (4.5 INCHES)	(T84)
6	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 12.7 CM (5 INCHES)	(T85)
7	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 14.0 CM (5.5 INCHES)	(T86)
8	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 15.2 CM (6 INCHES)	(T87)

.....
ROW 16

COLUMN

1	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 17.8 CM (7 INCHES)	(T88)
2	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 20.3 CM (8 INCHES)	(T89)
3	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 22.9 CM (9 INCHES)	(T90)
4	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 25.4 CM (10 INCHES)	(T91)
5	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 27.9 CM (11 INCHES)	(T92)
6	* FLOOR TEMP CELL #4 PROBE #3 (NW) AT 30.5 CM (12 INCHES)	(T93)
7	* FLOOR TEMP CELL #4 PROBE #3 (NW) AT 35.6 CM (14 INCHES)	(T94)
8	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 40.6 CM (16 INCHES)	(T95)

.....
ROW 17

COLUMN

1	* FLOOR TEMP CELL #4 PROBE #3 (NW) AT 45.7 CM (18 INCHES)	(T96)
2	FLOOR TEMP CELL #4 PROBE #3 (NW) AT 55.9 CM (22 INCHES)	(T98)
3	S FOUNDATION INSIDE TEMP CELL #4 0 CM BELOW SLAB	(T101)
4	S FOUNDATION INSIDE TEMP CELL #4 10 CM BELOW SLAB	(T102)
5	S FOUNDATION INSIDE TEMP CELL #4 20 CM BELOW SLAB	(T103)
6	S FOUNDATION INSIDE TEMP CELL #4 31 CM BELOW SLAB	(T104)
7	S FOUNDATION INSIDE TEMP CELL #4 41 CM BELOW SLAB	(T105)
8	S FOUNDATION INSIDE TEMP CELL #4 51 CM BELOW SLAB	(T106)

.....
ROW 18

COLUMN

1	S FOUNDATION INSIDE TEMP CELL #4 61 CM BELOW SLAB	(T107)
2	S FOUNDATION OUTSIDE TEMP CELL #4 0 CM BELOW SLAB	(T108)
3	S FOUNDATION OUTSIDE TEMP CELL #4 20 CM BELOW SLAB	(T109)
4	S FOUNDATION OUTSIDE TEMP CELL #4 41 CM BELOW SLAB	(T110)
5	S FOUNDATION OUTSIDE TEMP CELL #4 61 CM BELOW SLAB	(T111)
6	S FNDTN INSULATION OUTER SURF TEMP CELL #4 0 CM BELOW SLAB	(T112)
7	S FNDTN INSULATION OUTER SURF TEMP CELL #4 10 CM BELOW SLAB	(T113)
8	S FNDTN INSULATION OUTER SURF TEMP CELL #4 20 CM BELOW SLAB	(T114)

.....
ROW 19

COLUMN

1	S FNDTN INSULATION OUTER SURF TEMP CELL #4 31 CM BELOW SLAB	(T115)
2	S FNDTN INSULATION OUTER SURF TEMP CELL #4 41 CM BELOW SLAB	(T116)
3	S FNDTN INSULATION OUTER SURF TEMP CELL #4 51 CM BELOW SLAB	(T117)
4	S FNDTN INSULATION OUTER SURF TEMP CELL #4 61 CM BELOW SLAB	(T118)
5	E FOUNDATION INSIDE TEMP CELL #4 0 CM BELOW SLAB	(T119)
6	E FOUNDATION INSIDE TEMP CELL #4 10 CM BELOW SLAB	(T120)
7	E FOUNDATION INSIDE TEMP CELL #4 20 CM BELOW SLAB	(T121)
8	E FOUNDATION INSIDE TEMP CELL #4 31 CM BELOW SLAB	(T122)

.....

ROW 20

COLUMN

1	E FOUNDATION INSIDE TEMP CELL #4 41 CM BELOW SLAB	(T123)
2	E FOUNDATION INSIDE TEMP CELL #4 51 CM BELOW SLAB	(T124)
3	E FOUNDATION INSIDE TEMP CELL #4 61 CM BELOW SLAB	(T125)
4	E FOUNDATION OUTSIDE TEMP CELL #4 0 CM BELOW SLAB	(T126)
5	E FOUNDATION OUTSIDE TEMP CELL #4 20 CM BELOW SLAB	(T127)
6	E FOUNDATION OUTSIDE TEMP CELL #4 41 CM BELOW SLAB	(T128)
7	E FOUNDATION OUTSIDE TEMP CELL #4 61 CM BELOW SLAB	(T129)
8	E FNDTN INSULATION OUTER SURF TEMP CELL #4 0 CM BELOW SLAB	(T130)

.....

ROW 21

COLUMN

1	E FNDTN INSULATION OUTER SURF TEMP CELL #4 10 CM BELOW SLAB	(T131)
2	E FNDTN INSULATION OUTER SURF TEMP CELL #4 20 CM BELOW SLAB	(T132)
3	E FNDTN INSULATION OUTER SURF TEMP CELL #4 31 CM BELOW SLAB	(T133)
4	E FNDTN INSULATION OUTER SURF TEMP CELL #4 41 CM BELOW SLAB	(T134)
5	E FNDTN INSULATION OUTER SURF TEMP CELL #4 51 CM BELOW SLAB	(T135)
6	E FNDTN INSULATION OUTER SURF TEMP CELL #4 61 CM BELOW SLAB	(T136)
7	N FOUNDATION INSIDE TEMP CELL #4 0 CM BELOW SLAB	(T137)
8	N FOUNDATION INSIDE TEMP CELL #4 10 CM BELOW SLAB	(T138)

.....

ROW 22

COLUMN

1	N FOUNDATION INSIDE TEMP CELL #4 20 CM BELOW SLAB	(T139)
2	N FOUNDATION INSIDE TEMP CELL #4 31 CM BELOW SLAB	(T140)
3	N FOUNDATION INSIDE TEMP CELL #4 41 CM BELOW SLAB	(T141)
4	N FOUNDATION INSIDE TEMP CELL #4 51 CM BELOW SLAB	(T142)
5	N FOUNDATION INSIDE TEMP CELL #4 61 CM BELOW SLAB	(T143)
6	N FOUNDATION OUTSIDE TEMP CELL #4 0 CM BELOW SLAB	(T144)
7	N FOUNDATION OUTSIDE TEMP CELL #4 20 CM BELOW SLAB	(T145)
8	N FOUNDATION OUTSIDE TEMP CELL #4 41 CM BELOW SLAB	(T146)

.....

ROW 23

COLUMN

1	N FOUNDATION OUTSIDE TEMP CELL #4 61 CM BELOW SLAB	(T147)
2	N FNDTN INSULATION OUTER SURF TEMP CELL #4 0 CM BELOW SLAB	(T148)
3	N FNDTN INSULATION OUTER SURF TEMP CELL #4 10 CM BELOW SLAB	(T149)
4	N FNDTN INSULATION OUTER SURF TEMP CELL #4 20 CM BELOW SLAB	(T150)
5	N FNDTN INSULATION OUTER SURF TEMP CELL #4 31 CM BELOW SLAB	(T151)
6	N FNDTN INSULATION OUTER SURF TEMP CELL #4 41 CM BELOW SLAB	(T152)
7	N FNDTN INSULATION OUTER SURF TEMP CELL #4 51 CM BELOW SLAB	(T153)
8	N FNDTN INSULATION OUTER SURF TEMP CELL #4 61 CM BELOW SLAB	(T154)

.....

ROW 24

COLUMN

1	STRGE WALL SURF TEMP 69 CM W OF CENTER LINE 203 CM FRM FLOOR	(T155)
2	STRGE WALL SURF TEMP 69 CM W OF CENTER LINE 122 CM FRM FLOOR	(T156)
3	STRGE WALL SURF TEMP 69 CM W OF CENTER LINE 41 CM FRM FLOOR	(T157)
4	STRGE WALL SURF TEMP ON CENTER LINE 203 CM FRM FLOOR	(T158)
5	STRGE WALL SURF TEMP ON CENTER LINE 122 CM FRM FLOOR	(T159)
6	STRGE WALL SURF TEMP ON CENTER LINE 41 CM FRM FLOOR	(T160)
7	STRGE WALL SURF TEMP 69 CM E OF CENTER LINE 203 CM FRM FLOOR	(T161)
8	STRGE WALL SURF TEMP 69 CM E OF CENTER LINE 122 CM FRM FLOOR	(T162)

.....

ROW 25

COLUMN

1	STRGE WALL SURF TEMP 69 CM E OF CENTER LINE 41 CM FRM FLOOR	(T163)
2	STRGE WALL PROBE 0.32 CM FROM INNER SURFACE	(T164)
3	STRGE WALL PROBE 2.22 CM FROM INNER SURFACE	(T165)
4	STRGE WALL PROBE 6.03 CM FROM INNER SURFACE	(T166)
5	STRGE WALL PROBE 9.84 CM FROM INNER SURFACE	(T167)
6	STRGE WALL PROBE 13.65 CM FROM INNER SURFACE	(T168)
7	STRGE WALL PROBE 17.46 CM FROM INNER SURFACE	(T169)
8	STRGE WALL PROBE 19.05 CM FROM INNER SURFACE	(T170)

.....

ROW 26

COLUMN

1	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 10 CM FROM FLOOR	(T171)
2	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 20 CM FROM FLOOR	(T172)
3	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 30 CM FROM FLOOR	(T173)
4	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 76 CM FROM FLOOR	(T174)
5	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 122 CM FROM FLOOR	(T175)
6	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 168 CM FROM FLOOR	(T176)
7	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 213 CM FROM FLOOR	(T177)
8	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 224 CM FROM FLOOR	(T178)

.....

ROW 27

COLUMN

1	AIR TEMP CELL #4 275 CM FROM SOUTH WALL 234 CM FROM FLOOR	(T179)
2	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 10 CM FROM FLOOR	(T180)
3	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 20 CM FROM FLOOR	(T181)
4	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 30 CM FROM FLOOR	(T182)
5	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 79 CM FROM FLOOR	(T183)
6	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 127 CM FROM FLOOR	(T184)
7	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 175 CM FROM FLOOR	(T185)
8	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 224 CM FROM FLOOR	(T186)

.....

ROW 28

COLUMN

1	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 272 CM FROM FLOOR	(T187)
2	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 320 CM FROM FLOOR	(T188)
3	AIR TEMP CELL #4 580 CM FROM SOUTH WALL 368 CM FROM FLOOR	(T189)
4	BLACK GLOBE TEMP CELL #4 152 CM FRM S WALL 152 CM FRM FLOOR	(T190)
5	BLACK GLOBE TEMP CELL #4 472 CM FRM S WALL 152 CM FRM FLOOR	(T191)
6	BLACK GLOBE TEMP CELL #4 700 CM FRM S WALL 152 CM FRM FLOOR	(T192)
7	AIR TEMP CELL #3 (5 PT AVER 3 OF N STRING & 2 OF S STRING) N STRING 326 CM FRM FLOOR 66 CM FRM E WALL 579 CM FRM S WAL 187 CM FRM FLOOR 66 CM FRM E WALL 579 CM FRM S WAL 74 CM FRM FLOOR 66 CM FRM E WALL 579 CM FRM S WAL	(T193)
8	AIR TEMP CELL #4 15 CM FROM CLRSTY 30 CM FROM ROOF PEAK	(T194)

.....

ROW 29

COLUMN

1	AIR TEMP CELL #4 15 CM FROM CLRSTY 20 CM FROM ROOF PEAK	(T195)
2	AIR TEMP CELL #4 15 CM FROM CLRSTY 10 CM FROM ROOF PEAK	(T196)
3	EAST WALL OUTER SURF TEMP CELL #4 SOUTH SECTION	(T197)
4	EAST WALL OUTER SURF TEMP CELL #4 NORTH SECTION	(T198)
5	NORTH WALL OUTER SURF TEMP CELL #4	(T199)
6	AIR TEMP CELL #3 N SECT 275 CM FRM FLOOR 66 CM FRM E WALL 589 CM FROM SOUTH WALL	(T251)
7	AIR TEMP CELL #3 N SECT 49 CM FRM FLOOR 66 CM FRME WALL 589 CM FROM SOUTH WALL	(T252)
8	SURF TEMP OF HEAT FLUX SENSOR #222	(T253)

.....

ROW 30

COLUMN

1	SURF TEMP OF HEAT FLUX SENSOR #220	(T254)
2	SURF TEMP OF HEAT FLUX SENSOR #221	(T255)
3	SURF TEMP OF HEAT FLUX SENSOR #227	(T256)
4	SURF TEMP OF HEAT FLUX SENSOR #228	(T257)
5	SURF TEMP OF HEAT FLUX SENSOR #226	(T258)
6	SURF TEMP OF HEAT FLUX SENSOR #225	(T259)
7	SURF TEMP OF HEAT FLUX SENSOR #223	(T260)
8	SURF TEMP OF HEAT FLUX SENSOR #224	(T261)

.....

ROW 31

COLUMN

1	SURF TEMP OF HEAT FLUX SENSOR #229	(T262)
2	SURF TEMP OF HEAT FLUX SENSOR #230	(T264)
3	HEATER DISCHARGE TEMP, CELL #4	(T265)
4	PINK GLOBE TEMP CELL #4 472 CM FR S WALL 152 CM FR FLOOR	(T512)
5	PINK GLOBE TEMP CELL #4 152 CM FR S WALL 152 CM FR FLOOR	(T513)
6	OUTSIDE TEMP - MECH ASPIRATED- SOUTH	(T514)
7	OUTSIDE TEMP - MECH ASPIRATED- NORTH	(T515)
8	BLACK GLOBE TEMP CELL 4 580 CM FR S WALL 152 CM FR FLOOR	(T516)

.....

ROW 32

COLUMN

1	BLACK GLOBE TEMP CELL 4 275 CM FR S WALL 152 CM FR FLOOR	(T517)
2	AIR TEMP CELL #4 700 CM FROM S WALL 152 CM FROM FLOOR	(T518)
3	AIR TEMP CELL#4 472 CM FROM S WALL 152 CM FROM FLOOR	(T519)
4	AIR TEMP CELL#4 152 CM FROM S WALL 152 CM FROM FLOOR	(T520)
5	GROUND TEMP PROBE CELL #2. 297 CM FROM BELOW FLOOR 391 CM FROM S WALL 144 CM FROM W WALL	(T277)
6	GROUND TEMP PROBE CELL #2. 269 CM FROM BELOW FLOOR 391 CM FROM S WALL 144 CM FROM W WALL	(T278)
7	GROUND TEMP PROBE CELL #2. 239 CM FROM BELOW FLOOR 391 CM FROM S WALL 144 CM FROM W WALL	(T279)
8	GROUND TEMP PROBE CELL #2. 208 CM FROM BELOW FLOOR 391 CM FROM S WALL 144 CM FROM W WALL	(T280)

.....

ROW 33

COLUMN

1	GROUND TEMP PROBE CELL #2. 178 CM FROM BELOW FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T281)
2	GROUND TEMP PROBE CELL #2. 148 CM FROM BELOW FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T282)
3	GROUND TEMP PROBE CELL #2. 87 CM FROM BELOW FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T283)
4	GROUND TEMP PROBE CELL #2. 55 CM FROM BELOW FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T284)
5	* GROUND TEMP PROBE CELL #2. 26 CM FROM BELOW FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T285)
6	GROUND TEMP PROBE CELL #2. 4 CM ABOVE FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T286)
7	GROUND TEMP PROBE CELL #2. 35 CM ABOVE FLOOR 391 CM FROM SOUTH WALL 144 CM FROM W WALL	(T287)
8	TROMBE WALL PROBE 1 PT. 1. 19.05 CM FROM INSIDE SURFACE	(T288)

.....

ROW 34

COLUMN

1	TROMBE WALL PROBE 1 PT. 2. 17.46 CM FROM INSIDE SURFACE	(T289)
2	TROMBE WALL PROBE 1 PT. 3. 13.65 CM FROM INSIDE SURFACE	(T290)
3	TROMBE WALL PROBE 1 PT. 4. 9.84 CM FROM INSIDE SURFACE	(T291)
4	TROMBE WALL PROBE 1 PT. 5. 6.03 CM FROM INSIDE SURFACE	(T292)
5	TROMBE WALL PROBE 1 PT. 6. 3.22 CM FROM INSIDE SURFACE	(T293)
6	TROMBE WALL PROBE 1 PT. 7. 0.32 CM FROM INSIDE SURFACE	(T294)
7	TROMBE WALL PROBE 2 PT. 1. 19.05 CM FROM INSIDE SURFACE	(T295)
8	TROMBE WALL PROBE 2 PT. 2. 17.46 CM FROM INSIDE SURFACE	(T296)

.....

ROW 35

COLUMN

1	TROMBE WALL PROBE 2 PT. 3. 13.65 CM FROM INSIDE SURFACE	(T297)
2	TROMBE WALL PROBE 2 PT. 4. 9.84 CM FROM INSIDE SURFACE	(T298)
3	TROMBE WALL PROBE 2 PT. 5. 6.03 CM FROM INSIDE SURFACE	(T299)
4	TROMBE WALL PROBE 2 PT. 6. 2.22 CM FROM INSIDE SURFACE	(T300)
5	TROMBE WALL PROBE 2 PT. 7. 0.32 CM FROM INSIDE SURFACE	(T301)
6	TROMBE WALL PROBE 3 PT. 1. 19.05 CM FROM INSIDE SURFACE	(T302)
7	TROMBE WALL PROBE 3 PT. 2. 17.46 CM FROM INSIDE SURFACE	(T303)
8	TROMBE WALL PROBE 3 PT. 3. 13.65 CM FROM INSIDE SURFACE	(T304)

.....

ROW 36

COLUMN

1	* TROMBE WALL PROBE 3 PT. 4. 9.84 CM FROM INSIDE SURFACE	(T305)
2	TROMBE WALL PROBE 3 PT. 5. 6.03 CM FROM INSIDE SURFACE	(T306)
3	TROMBE WALL PROBE 3 PT. 6. 2.22 CM FROM INSIDE SURFACE	(T307)
4	TROMBE WALL PROBE 3 PT. 7. 0.32 CM FROM INSIDE SURFACE	(T308)
5	TROMBE WALL PROBE 4 PT. 1. 19.05 CM FROM INSIDE SURFACE	(T309)
6	TROMBE WALL PROBE 4 PT. 2. 17.46 CM FROM INSIDE SURFACE	(T310)
7	TROMBE WALL PROBE 4 PT. 3. 13.56 CM FROM INSIDE SURFACE	(T311)
8	TROMBE WALL PROBE 4 PT. 4. 9.84 CM FROM INSIDE SURFACE	(T312)

.....

ROW 37

COLUMN

1	TROMBE WALL PROBE 4 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T313)
2	TROMBE WALL PROBE 4 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T314)
3	TROMBE WALL PROBE 4 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T315)
4	TROMBE WALL PROBE 5 PT. 1.	19.05 CM FROM INSIDE SURFACE	(T316)
5	TROMBE WALL PROBE 5 PT. 2.	17.46 CM FROM INSIDE SURFACE	(T317)
6	TROMBE WALL PROBE 5 PT. 3.	13.65 CM FROM INSIDE SURFACE	(T318)
7	TROMBE WALL PROBE 5 PT. 4.	9.84 CM FROM INSIDE SURFACE	(T319)
8	TROMBE WALL PROBE 5 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T320)

.....

ROW 38

COLUMN

1	TROMBE WALL PROBE 5 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T321)
2	TROMBE WALL PROBE 5 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T322)
3	* TROMBE WALL PROBE 6 PT. 1.	19.05 CM FROM INSIDE SURFACE	(T323)
4	TROMBE WALL PROBE 6 PT. 2.	17.46 CM FROM INSIDE SURFACE	(T324)
5	TROMBE WALL PROBE 6 PT. 3.	13.65 CM FROM INSIDE SURFACE	(T325)
6	TROMBE WALL PROBE 6 PT. 4.	9.84 CM FROM INSIDE SURFACE	(T326)
7	TROMBE WALL PROBE 6 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T327)
8	TROMBE WALL PROBE 6 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T328)

.....

ROW 39

COLUMN

1	TROMBE WALL PROBE 6 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T329)
2	TROMBE WALL PROBE 7 PT. 1.	19.05 CM FROM INSIDE SURFACE	(T330)
3	TROMBE WALL PROBE 7 PT. 2.	17.46 CM FROM INSIDE SURFACE	(T331)
4	TROMBE WALL PROBE 7 PT. 3.	13.65 CM FROM INSIDE SURFACE	(T332)
5	* TROMBE WALL PROBE 7 PT. 4.	9.84 CM FROM INSIDE SURFACE	(T333)
6	TROMBE WALL PROBE 7 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T334)
7	TROMBE WALL PROBE 7 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T335)
8	TROMBE WALL PROBE 7 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T336)

.....

ROW 40

COLUMN

1	TROMBE WALL PROBE 8 PT. 1.	19.05 CM FROM INSIDE SURFACE	(T337)
2	TROMBE WALL PROBE 8 PT. 2.	17.46 CM FROM INSIDE SURFACE	(T338)
3	TROMBE WALL PROBE 8 PT. 3.	13.65 CM FROM INSIDE SURFACE	(T339)
4	TROMBE WALL PROBE 8 PT. 4.	9.84 CM FROM INSIDE SURFACE	(T340)
5	TROMBE WALL PROBE 8 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T341)
6	TROMBE WALL PROBE 8 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T342)
7	TROMBE WALL PROBE 8 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T343)
8	TROMBE WALL PROBE 9 PT. 1.	19.05 CM FROM INSIDE SURFACE	(T344)

.....

ROW 41

COLUMN

1	* TROMBE WALL PROBE 9 PT. 2.	17.46 CM FROM INSIDE SURFACE	(T345)
2	TROMBE WALL PROBE 9 PT. 3.	13.65 CM FROM INSIDE SURFACE	(T346)
3	TROMBE WALL PROBE 9 PT. 4.	9.84 CM FROM INSIDE SURFACE	(T347)
4	TROMBE WALL PROBE 9 PT. 5.	6.03 CM FROM INSIDE SURFACE	(T348)
5	* TROMBE WALL PROBE 9 PT. 6.	2.22 CM FROM INSIDE SURFACE	(T349)
6	TROMBE WALL PROBE 9 PT. 7.	0.32 CM FROM INSIDE SURFACE	(T350)
7	AIR TEMP CELL #2 NEAR THERMOSTAT ON WEST WALL		(T400)
8	INSIDE GLAZING SURFACE TEMP 302 CM FROM EAST WALL		(T401)

.....

ROW 42

COLUMN

1	INSIDE GLAZING SURFACE TEMP 180 CM FROM EAST WALL	(T402)
2	INSIDE GLAZING SURFACE TEMP 71 CM FROM EAST WALL	(T403)
3	OUTSIDE T-WALL SURFACE TEMP 302 CM FROM EAST WALL	(T404)
4	OUTSIDE T-WALL SURFACE TEMP 180 CM FROM EAST WALL	(T405)
5	OUTSIDE T-WALL SURFACE TEMP 71 CM FROM EAST WALL	(T406)
6	UPPER WEST SIDE VENT AIR TEMP IN TROMBE WALL	(T407)
7	LOWER WEST SIDE VENT AIR TEMP IN TROMBE WALL	(T408)
8	UPPER EAST SIDE VENT AIR TEMP IN TROMBE WALL	(T409)

.....

ROW 43

COLUMN

1	LOWER EAST SIDE VENT AIR TEMP IN TROMBE WALL	(T410)
2	OUTSIDE AIR TEMP NORTH SIDE (MECH ASPIRATED SHIELD)	(T411)
3	AIR TEMP CELL #2 580 CM FROM S WALL 10 CM FROM FLOOR	(T412)
4	AIR TEMP CELL #2 580 CM FROM S WALL 20 CM FROM FLOOR	(T413)
5	AIR TEMP CELL #2 580 CM FROM S WALL 30 CM FROM FLOOR	(T414)
6	AIR TEMP CELL #2 580 CM FROM S WALL 80 CM FROM FLOOR	(T415)
7	AIR TEMP CELL #2 580 CM FROM S WALL 127 CM FROM FLOOR	(T416)
8	AIR TEMP CELL #2 580 CM FROM S WALL 175 CM FROM FLOOR	(T417)

.....

ROW 44

COLUMN

1	AIR TEMP CELL #2 580 CM FROM S WALL 224 CM FROM FLOOR	(T418)
2	AIR TEMP CELL #2 580 CM FROM S WALL 272 CM FROM FLOOR	(T419)
3	AIR TEMP CELL #2 580 CM FROM S WALL 320 CM FROM FLOOR	(T420)
4	AIR TEMP CELL #2 580 CM FROM S WALL 368 CM FROM FLOOR	(T421)
5	AIR TEMP CELL #2 275 CM FROM S WALL 10 CM FROM FLOOR	(T422)
6	AIR TEMP CELL #2 275 CM FROM S WALL 20 CM FROM FLOOR	(T423)
7	AIR TEMP CELL #2 275 CM FROM S WALL 30 CM FROM FLOOR	(T424)
8	AIR TEMP CELL #2 275 CM FROM S WALL 76 CM FROM FLOOR	(T425)

.....

ROW 45

COLUMN

1	AIR TEMP CELL #2 275 CM FROM S WALL 122 CM FROM FLOOR	(T426)
2	AIR TEMP CELL #2 275 CM FROM S WALL 168 CM FROM FLOOR	(T427)
3	AIR TEMP CELL #2 275 CM FROM S WALL 213 CM FROM FLOOR	(T428)
4	AIR TEMP CELL #2 275 CM FROM S WALL 224 CM FROM FLOOR	(T429)
5	AIR TEMP CELL #2 275 CM FROM S WALL 234 CM FROM FLOOR	(T430)
6	SLOPED CEIL TEMP 97 CM FROM CLRSTRY 122 CM W OF CENTER LINE	(T431)
7	* SLOPED CEIL TEMP 97 CM FROM CLRSTRY ON CENTER LINE	(T432)
8	SLOPED CEIL TEMP 97 CM FROM CLRSTRY 122 CM E OF CENTER LINE	(T433)

.....

ROW 46

COLUMN

1	SLOPED CEIL TEMP 290 CM FROM CLRSTRY 122 CM W OF CENTER LINE	(T434)
2	SLOPED CEIL TEMP 290 CM FROM CLRSTRY ON CENTER LINE	(T435)
3	SLOPED CEIL TEMP 290 CM FROM CLRSTRY 122 CM E OF CENTER LINE	(T436)
4	FLAT CEIL TEMP 122 CM FROM S WALL 122 CM W OF CENTER LINE	(T437)
5	FLAT CEIL TEMP 122 CM FROM S WALL ON CENTER LINE	(T438)
6	FLAT CEIL TEMP 122 CM FROM S WALL 122 CM E OF CENTER LINE	(T439)
7	FLAT CEIL TEMP 366 CM FROM S WALL 122 CM W OF CENTER LINE	(T440)
8	FLAT CEIL TEMP 366 CM FROM S WALL ON CENTER LINE	(T441)

.....

ROW 47

COLUMN

1	FLAT CEIL TEMP 366 CM FROM S WALL 122 CM E OF CENTER LINE	(T442)
2	FLOOR SURFACE TEMP 102 CM FROM S WALL 122 CM W OF CENTER LINE	(T443)
3	FLOOR SURFACE TEMP 102 CM FROM S WALL ON CENTER LINE	(T444)
4	FLOOR SURFACE TEMP 102 CM FROM S WALL 122 CM E OF CENTER LINE	(T445)
5	FLOOR SURFACE TEMP 307 CM FROM S WALL 122 CM E OF CENTER LINE	(T446)
6	FLOOR SURFACE TEMP 307 CM FROM S WALL ON CENTER LINE	(T447)
7	FLOOR SURFACE TEMP 307 CM FROM S WALL 122 CM W OF CENTER LINE	(T448)
8	FLOOR SURFACE TEMP 513 CM FROM S WALL 122 CM W OF CENTER LINE	(T449)

.....

ROW 48

COLUMN

1	FLOOR SURFACE TEMP 513 CM FROM S WALL ON CENTER LINE	(T450)
2	FLOOR SURFACE TEMP 513 CM FROM S WALL 122 CM E OF CENTER LINE	(T451)
3	FLOOR SURFACE TEMP 719 CM FROM S WALL 122 CM W OF CENTER LINE	(T452)
4	FLOOR SURFACE TEMP 719 CM FROM S WALL ON CENTER LINE	(T453)
5	FLOOR SURFACE TEMP 719 CM FROM S WALL 122 CM E OF CENTER LINE	(T454)
6	BLACK GLOBE TEMP CELL #2 152 CM FRM S WALL 152 CM FRM FLOOR	(T455)
7	BLACK GLOBE TEMP CELL #2 472 CM FRM S WALL 152 CM FRM FLOOR	(T456)
8	BLACK GLOBE TEMP CELL #2 700 CM FRM S WALL 152 CM FRM FLOOR	(T457)

.....

ROW 49

COLUMN

1	OUTSIDE AIR TEMP SOUTH SIDE (MECH ASPIRATED SHIELD)	(T458)
2	T-WALL INSIDE SURF TEMP 20 CM FRM E WALL 211.0 CM FRM FLOOR	(T459)
3	T-WALL INSIDE SURF TEMP 20 CM FRM E WALL 124.5 CM FRM FLOOR	(T460)
4	T-WALL INSIDE SURF TEMP 20 CM FRM E WALL 23.0 CM FRM FLOOR	(T461)
5	T-WALL INSIDE SURF TEMP 180 CM FRM E WALL 211.0 CM FRM FLOOR	(T462)
6	T-WALL INSIDE SURF TEMP 180 CM FRM E WALL 124.5 CM FRM FLOOR	(T463)
7	T-WALL INSIDE SURF TEMP 180 CM FRM E WALL 23.0 CM FRM FLOOR	(T464)
8	T-WALL INSIDE SURF TEMP 353 CM FRM E WALL 211.0 CM FRM FLOOR	(T465)

.....

ROW 50

COLUMN

1	T-WALL INSIDE SURF TEMP 353 CM FRM E WALL 124.5 CM FRM FLOOR	(T466)
2	T-WALL INSIDE SURF TEMP 353 CM FRM E WALL 23.0 CM FRM FLOOR	(T467)
3	E WALL CELL #2 SURF TEMP 163 CM FRM S WALL 120 CM FRM FLOOR	(T468)
4	E WALL CELL #2 SURF TEMP 582 CM FRM S WALL 310 CM FRM FLOOR	(T469)
5	E WALL CELL #2 SURF TEMP 582 CM FRM S WALL 132 CM FRM FLOOR	(T470)
6	N WALL CELL #2 SURF TEMP 96.5 CM FR E WALL 206 CM FRM FLOOR	(T471)
7	N WALL CELL #2 SURF TEMP 96.5 CM FR E WALL 120 CM FRM FLOOR	(T472)
8	N WALL CELL #2 SURF TEMP 290.0 CM FR E WALL 218 CM FRM FLOOR	(T473)

.....

ROW 51

COLUMN

1	W WALL CELL #2 SURF TEMP 187 CM FRM S WALL 160 CM FRM FLOOR	(T474)
2	W WALL CELL #2 SURF TEMP 582 CM FRM S WALL 305 CM FRM FLOOR	(T475)
3	FLOOR SURF TEMP CELL #3, 7.61 CM FR N WALL ON CENTER LINE	(T476)
4	FLOOR SURF TEMP CELL #3, 15.24 CM FR N WALL ON CENTER LINE	(T477)
5	FLOOR SURF TEMP CELL #3, 30.48 CM FR N WALL ON CENTER LINE	(T478)
6	FLOOR SURF TEMP CELL #3, 60.96 CM FR N WALL ON CENTER LINE	(T479)
7	FLOOR SURF TEMP CELL #3, 101 CM FR N WALL ON CENTER LINE	(T480)
8	FLOOR SURF TEMP CELL #3, 317 CM FR N WALL ON CENTER LINE	(T481)

.....

ROW 52

COLUMN

1	FLOOR SURF TEMP CELL #3. 513 CM FR N WALL ON CENTER LINE	(T482)
2	FLOOR SURF TEMP CELL #3. 104 CM FR S WALL ON CENTER LINE	(T483)
3	FLOOR SURF TEMP CELL #3. 61 CM FR S WALL ON CENTER LINE	(T484)
4	FLOOR SURF TEMP CELL #3. 30.5 CM FR S WALL ON CENTER LINE	(T485)
5	FLOOR SURF TEMP CELL #3. 15.5 CM FR S WALL ON CENTER LINE	(T486)
6	FLOOR SURF TEMP CELL #3. 7.6 CM FR S WALL ON CENTER LINE	(T487)
7	FLOOR SURF TEMP CELL #3. 101.6 CM FR NORTH WALL 122 CM EAST OF CENTER LINE	(T488)
8	FLOOR SURF TEMP CELL #3. 317 CM FR NORTH WALL 122 CM EAST OF CENTER LINE	(T489)

.....

ROW 53

COLUMN

1	FLOOR SURF TEMP CELL #3. 513 CM FR NORTH WALL 122 CM EAST OF CENTER LINE	(T490)
2	FLOOR SURF TEMP CELL #3. 104 CM FR SOUTH WALL 122 CM EAST OF CENTER LINE	(T491)
3	FLOOR SURF TEMP CELL #3. 101 CM FR NORTH WALL 122 CM WEST OF CENTER LINE	(T492)
4	FLOOR SURF TEMP CELL #3. 317 CM FR NORTH WALL 122 CM WEST OF CENTER LINE	(T493)
5	FLOOR SURF TEMP CELL #3. 513 CM FR NORTH WALL 122 CM WEST OF CENTER LINE	(T494)
6	FLOOR SURF TEMP CELL #3. 102 CM FR SOUTH WALL 122 CM WEST OF CENTER LINE	(T495)
7	WEST WALL SURF TEMP CELL #2. 582 CM FR SOUTH WALL 125 CM ABOVE FLOOR	(T496)
8	AIR TEMP CELL #2. 152 CM FR SOUTH WALL 152 CM ABOVE FLOOR NEAR SOUTH BLACK GLOBE	(T497)

.....

ROW 54

COLUMN

1	AIR TEMP CELL #2. 472 CM FR SOUTH WALL 152 CM ABOVE FLOOR NEAR CENTER BLACK GLOBE	(T498)
2	AIR TEMP CELL #2. 700 CM FR SOUTH WALL 152 CM ABOVE FLOOR NEAR NORTH BLACK GLOBE	(T499)
3	OUTSIDE GROUND PROBE 298.5 CM BELOW GROUND	(T500)
4	OUTSIDE GROUND PROBE 270.0 CM BELOW GROUND	(T501)
5	* OUTSIDE GROUND PROBE 240.1 CM BELOW GROUND	(T502)
6	OUTSIDE GROUND PROBE 209.2 CM BELOW GROUND	(T503)
7	OUTSIDE GROUND PROBE 178.8 CM BELOW GROUND	(T504)
8	OUTSIDE GROUND PROBE 147.5 CM BELOW GROUND	(T505)

.....

ROW 55

COLUMN

1	OUTSIDE GROUND PROBE 117.5 CM BELOW GROUND	(T506)
2	OUTSIDE GROUNDPROBE 87.3 CM BELOW GROUND.	(T507)
3	OUTSIDE GROUNDPROBE 56.5 CM BELOW GROUND	(T508)
4	OUTSIDE GROUNDPROBE 26.5 CM BELOW GROUND	(T509)
5	OUTSIDE GROUND PROBE 4.4 CM ABOVE GROUND	(T510)
6	OUTSIDE GROUNDPROBE 35.0 CM ABOVE GROUND	(T511)
7	ENERGY USED BY THE FAN COIL UNIT IN CELL #2	(WH1)
8	ENERGY USED BY THE LIGHTS & OUTLETS IN CELL #2	(WH2)

.....

ROW 56

COLUMN

1	ENERGY USED BY THE FAN COIL UNIT IN CELL #3	(WH3)
2	ENERGY USED BY THE LIGHTS & OUTLETS IN CELL #3	(WH4)
3	ENERGY USED BY THE FAN COIL UNIT IN CELL #4	(WH5)
4	ENERGY USED BY THE LIGHTS & OUTLETS IN CELL #4	(WH6)
5	AIR INFILTRATION CELL #2	(VOLUME CHANGES PER HOUR)
6	AIR INFILTRATION CELL #3	(VOLUME CHANGES PER HOUR)
7	AIR INFILTRATION CELL #4	(VOLUME CHANGES PER HOUR)
8	NOT USED	(9999.99)

.....
.....

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET (See instructions)	1. PUBLICATION OR REPORT NO. NBSIR 84-2911	2. Performing Organ. Report No.	3. Publication Date August 1984
---	---	---------------------------------	------------------------------------

4. TITLE AND SUBTITLE

National Bureau of Standards Passive Solar Test Facility - Instrumentation and Site Handbook

5. AUTHOR(S)

Bal M. Mahajan

6. PERFORMING ORGANIZATION (If joint or other than NBS, see instructions) NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234	7. Contract/Grant No. 8. Type of Report & Period Covered
---	---

9. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP)

U.S. Dept. of Energy
 Office of Solar Heat Technologies
 Forrestal Building
 Washington, D.C. 20585

10. SUPPLEMENTARY NOTES

Document describes a computer program; SF-185, FIPS Software Summary, is attached.

11. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here)

The National Bureau of Standards (NBS), under the sponsorship of the U.S. Department of Energy (DoE) has constructed a passive solar test facility. As a part of the DoE's Experimental Systems Research Program, the NBS test facility has been constructed for the purpose of acquiring and distributing to participating researchers class A level performance data for different passive systems. These data are acquired for use in: detailed building energy analysis and model/algorithm validation; and performance characterization of passive subsystems.

This handbook provides a complete description of the test building, thermophysical properties of the building material, location of the sensors installed at the test facility, and data acquisition system and procedures.

12. KEY WORDS (Six to twelve entries; alphabetical order; capitalize only proper names; and separate key words by semicolons)

building, data acquisition, location; material; passive; property; sensor; solar; system test facility; thermophysical; wall section

13. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402. <input checked="" type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA. 22161	14. NO. OF PRINTED PAGES 88 15. Price \$11.50
--	--

